

Neobiotech
IMPLANT SYSTEM

**Neo
Biotech**
Satisfaction to Dentists

Butterfly

IMPLANT SYSTEM



Contents

IS Implant System

Neobiotch Product Line Up	4
IS Implant System Chart	7
IS-II active	8
IS-II active Fixture (S.L.A. Surface)	10
IS-III active Fixture (S.L.A. Surface)	13
IS Healing Abutment	14
IS Prosthetic Flow Chart (Abutment)	16
IS Transfer Impression Coping	17
IS Pick-up Impression Coping	18
IS Lab Analog	19
IS Temporary Abutment	20
IS Cemented Abutment	21
IS Angled Abutment	26
IS UCLA Abutment	28
IS Prosthetic Flow Chart (Multi Unit Abutment)	29
IS Multi Unit Abutment	30
IS Prosthetic Flow Chart (Ball Abutment)	32
IS Ball Abutment	33
Neobiotch Equator	35
Digital Solutions	36
Ti-Cylinder Abutment	37
Ti-Link Abutment	38
Surgical Guide Fixed	39

IT Implant System

IT Implant System Chart	41
IT-III active	42
IT-III active Fixture (S.L.A. Surface)	43
IT Healing Abutment	44
IT Prosthetic Flow Chart (Abutment)	44
IT Transfer Impression Coping	45
IT Pick-up Impression Coping	45
IT Lab Analog	45
IT Cemented Abutment	46
IT Angled Abutment	47
IT Collared Angled Abutment	48
IT UCLA Abutment	48

Neobiotch Surgical Kit

Neo Master Kit	51
Neo Master Kit Components	52
Neo Master Kit - Drilling Sequence	56
Neo NaviGuide Kit	57
Surgical Guide Sleeve	57
Ridge Wider Kit	58
Neo Surgical Accessory Kit	58

Neobiotch Prosthetic Kit

Neo Prosthetic Kit	59
Neo Prosthetic Planning Kit	59

Neobiotch Solution System

SCA Kit	61
SLA Kit	61
FR Kit	63
SR Kit	66
ACM	70
Peri-implantitis Solution	71
AnyCheck	72



Product Line Up

Congratulations! You have made an excellent choice.
Welcome to the Neobiotech family

Implant System



IS System



IT System



Neo Master Kit



Core Kit



S-narrow Kit



Neo NaviGuide Kit



Ridge Wider Kit



Accessory Kit



Prosthetic Kit



Neo Prosthetic Planning Kit

This catalog contains information of Neobiotech implant system only. To get information of other solution system, Please refer to Neo Solution catalogs.

Sinus Lift Solution



SCA Kit
(Sinus Crestal Approach Kit)



SLA Kit
(Sinus Lateral Approach Kit)

Repair Solution



FR Kit
(Fixture Remover Kit)



SR Kit
(Screw Remover Kit)

GBR Solution



ACM
(Auto Chip Maker)

Peri-implantitis Solution



i Brush
(Implant Brush)



iBrush2



R - Brush



T - Brush





























Neobiotech

IS IMPLANT SYSTEM


IS-II active / IS-III active

IS Implant System Chart

Fixture	Healing & Cover Screw	Abutment		Impression Coping	Lab Analog	
 IS-III active  IS-III active S-Wide  IS-II active  IS-II active S-Wide	 Healing Abutment  Cover Screw	Solid		 PickCap		
		Cemented		 Impression Cap		
		Angled		 Pick-up Hex SCRP®	 Fixture Level	
		Shapable		 Hex SCRP®		
		UCLA	Gold		 Non-Hex	 Abutment Level
			CCM		 Transfer Hex Non-Hex	
		Temporary		 Impression coping positioner		
Ball		 Clinical Retainer Housing	 Lab Retainer Housing	 Ball Lab Analog		

IS-II active



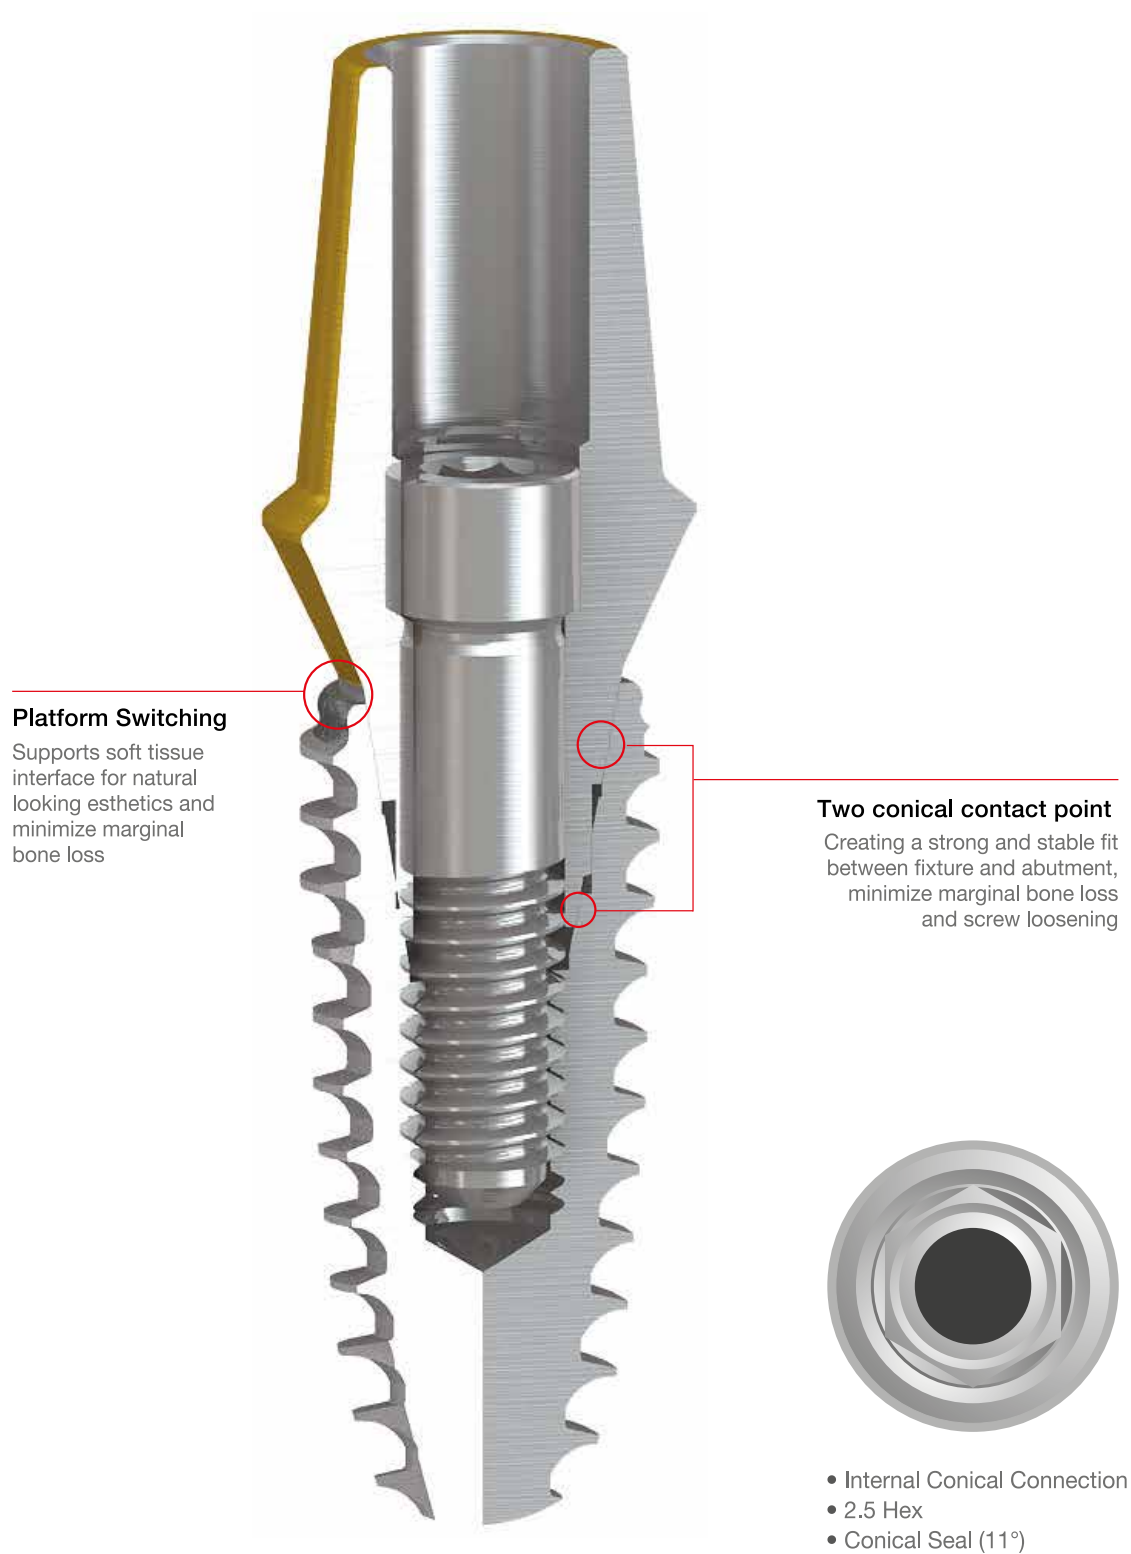


IS-II active Fixture (S.L.A. Surface)

The fixture bigger than Ø4.5 diameter is recommended to be placed in posterior area.

• Cover Screw included

Narrow / All 7.3mm Fixtures : ISN30S

Regular / Wide / S-Wide : ISC40S

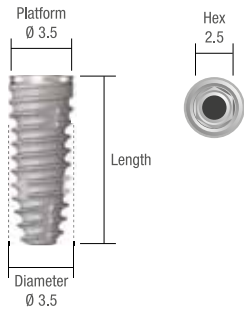


• Narrow / Diameter Ø 3.5



Length (mm)	8.5	10.0	11.5	13.0
Product name	BIS3508A	BIS3510A	BIS3511A	BIS3513A

* Cover Screw Included

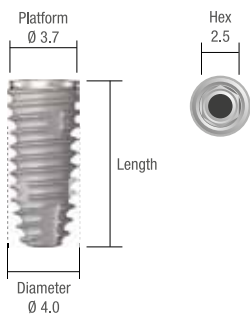


• Regular / Diameter Ø 4.0



Length (mm)	7.3	8.5	10.0	11.5	13.0
Product name	BIS4007A	BIS4008A	BIS4010A	BIS4011A	BIS4013A

* Cover Screw Included

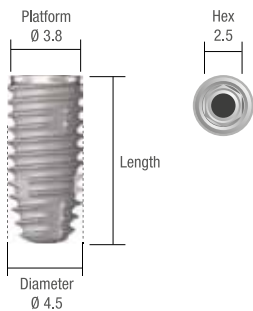


• Regular / Diameter Ø 4.5



Length (mm)	7.3	8.5	10.0	11.5	13.0
Product name	BIS4507A	BIS4508A	BIS4510A	BIS4511A	BIS4513A

* Cover Screw Included

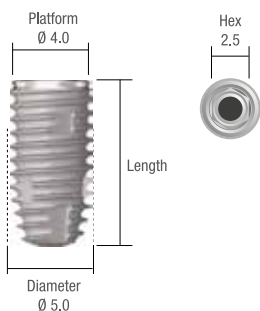

• Wide / Diameter Ø 5.0



Length (mm)	7.3	7.3	7.3	8.5	10.0	11.5	13.0
Product name	BIS5005A	BIS5006A	BIS5007A	BIS5008A	BIS5010A	BIS5011A	BIS5013A


* Cover Screw Included

** All measurements can be different with the actual size

IS-II active Fixture (S.L.A. Surface)

The fixture bigger than Ø4.5 diameter is recommended to be placed in posterior area.


• Cover Screw included



• S-Wide / Diameter Ø 5.5




Length(mm)	7.3	7.3	7.3	8.5	10.0	11.5	13.0
Product name	BIS5505A	BIS5506A	BIS5507A	BIS5508A	BIS5510A	BIS5511A	BIS5513A



• S-Wide / Diameter Ø 6.0



Length(mm)	7.3	8.5	10.0	11.5	13.0
Product name	BIS6007A	BIS6008A	BIS6010A	BIS6011A	BIS6013A



• S-Wide / Diameter Ø7.0




Length(mm)	7.3	8.5	10.0	11.5	13.0
Product name	BIS7007A	BIS7008A	BIS7010A	BIS7011A	BIS7013A


Requires S-Wide surgical kit for diameter Ø5.5 ~ Ø7.0 fixture
All measurements can be different with the actual size

Cover Screw

Narrow / All 7.3mm Fixtures



Regular / Wide / S-Wide

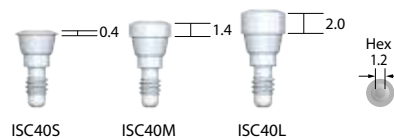

IS-III active

Micro Groove
Minimize bone loss and maintain bone level by treating superior area of fixture.

Micro Groove
Minimize bone loss and maintain bone level by treating superior area of fixture.

0.9 Pitch
Increase contact area between thread pitch and results in increasing of stability and osseointegration

S.L.A. Surface
Improvement of process technology of S.L.A surface

Magic Thread
Specially designed to endure vertical and lateral force

Apex
Excellent to both immediate placement and immediate loading

Wide Cutting Edge
Improvement of fixation and increase clinician's comfort when placing implants by widening cutting edge area

- Osteoconductivity Implant Surface (S.L.A.)
- Crestal MacroThread Design
- Self-Compactable Apex
- Powerful Deep Thread
- Micro Groove Design
- Conical Seal 11°


Cover Screw

S-Narrow



ISC25S*

Narrow



ISN30S




ISN30M



ISN30L



Regular / Wide



ISC40S



ISC40M



ISC40L




* This component is only for S-narrow fixture.

IS-III active Fixture (S.L.A. Surface)

The fixture bigger than Ø4.5 diameter is recommended to be placed in posterior area.

- Cover Screw Included Fixture product code
 fixture product code (ex : IS34010A)
 S-narrow : ISC25S / Narrow : ISN30S
 Regular / Wide / S-Wide : ISC40S


- Cover Screw Excluded Fixture product code
 fixture product code (ex : IS34010AP)

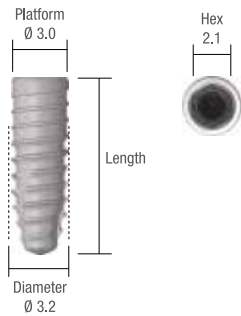

• S-Narrow / Diameter Ø 3.2




Length (mm)	8.5	10.0	11.5	13.0
Product name	IS3SN3008AP	IS3SN3010AP	IS3SN3011AP	IS3SN3013AP

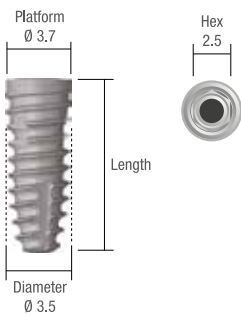

• Narrow / Diameter Ø 3.5




Length (mm)	8.5	10.0	11.5	13.0
Product name	IS33508A	IS33510A	IS33511A	IS33513A

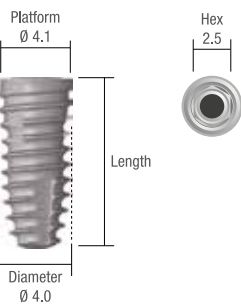

• Regular / Diameter Ø 4.0




Length (mm)	7.3	8.5	10.0	11.5	13.0
Product name	IS34007A	IS34008A	IS34010A	IS34011A	IS34013A

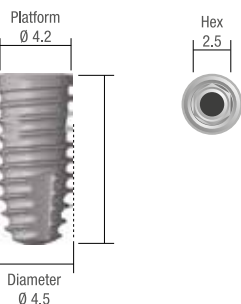

• Regular / Diameter Ø 4.5



Length (mm)	7.3	8.5	10.0	11.5	13.0
Product name	IS34507A	IS34508A	IS34510A	IS34511A	IS34513A

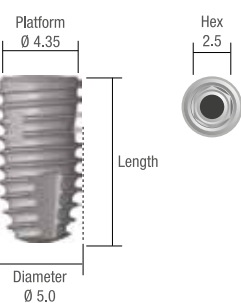

• Wide / Diameter Ø 5.0




Length (mm)	6.6	7.3	8.5	10.0	11.5	13.0
Product name	IS35006A	IS35007A	IS35008A	IS35010A	IS35011A	IS35013A

** All measurements can be different with the actual size

IS Healing Abutment

Temporary restorations for contouring of the soft tissue

- Tightening torque : 8~10 Ncm

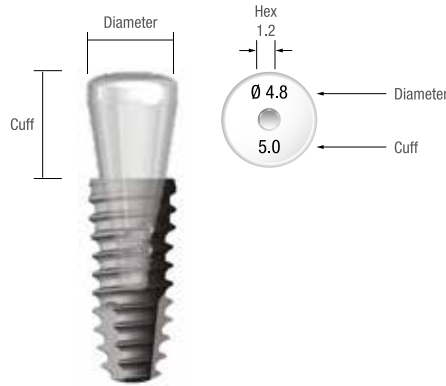

• Diameter Ø 3.0



Diameter	Ø 3.0	
Cuff (mm)	3.0	5.0
Product name	ISH3003 *	ISH3005 *

* These components are only for S-narrow fixture.


• Diameter Ø 3.8



Diameter	Ø 3.8	
Cuff (mm)	3.0	5.0
Product name	ISH3803 *	ISH3805 *


* These components are only for S-narrow fixture.

• Diameter Ø 4.0




Cuff (mm)	2.0	3.0	4.0	5.0	6.0
Product name	ISUH4002	ISUH4003	ISUH4004	ISUH4005	ISUH4006

• Diameter Ø 4.5



Cuff (mm)	2.0	3.0	4.0	5.0	6.0
Product name	ISUH4502	ISUH4503	ISUH4504	ISUH4505	ISUH4506

• Diameter Ø 4.8



Cuff (mm)	2.0	3.0	4.0	5.0	6.0	7.0
Product name	ISH402	ISH403	ISH404	ISH405	ISH406	ISH407

IS Healing Abutment



• Diameter Ø 5.5



Cuff (mm)	2.0	3.0	4.0	5.0	6.0	7.0
Product name	ISH502	ISH503	ISH504	ISH505	ISH506	ISH507



• Diameter Ø 6.0



Cuff (mm)	2.0	3.0	4.0	5.0	6.0	7.0
Product name	ISH602	ISH603	ISH604	ISH605	ISH606	ISH607



• Diameter Ø 6.8



Cuff (mm)	2.0	3.0	4.0	5.0	6.0	7.0
Product name	ISH702	ISH703	ISH704	ISH705	ISH706	ISH707



• Diameter Ø 8.0



Cuff (mm)	2.0	3.0	4.0	5.0	6.0	7.0
Product name	ISH802	ISH803	ISH804	ISH805	ISH806	ISH807

※ Ø 8.0, Ø 9.0 Healing Abutments are for Custom Abutment



• Diameter Ø 9.0




Cuff (mm)	2.0	3.0	4.0
Product name	ISH902	ISH903	ISH904

※ Ø 8.0, Ø 9.0 Healing Abutments are for Custom Abutment

Prosthetic Flow Chart

- IS Abutment

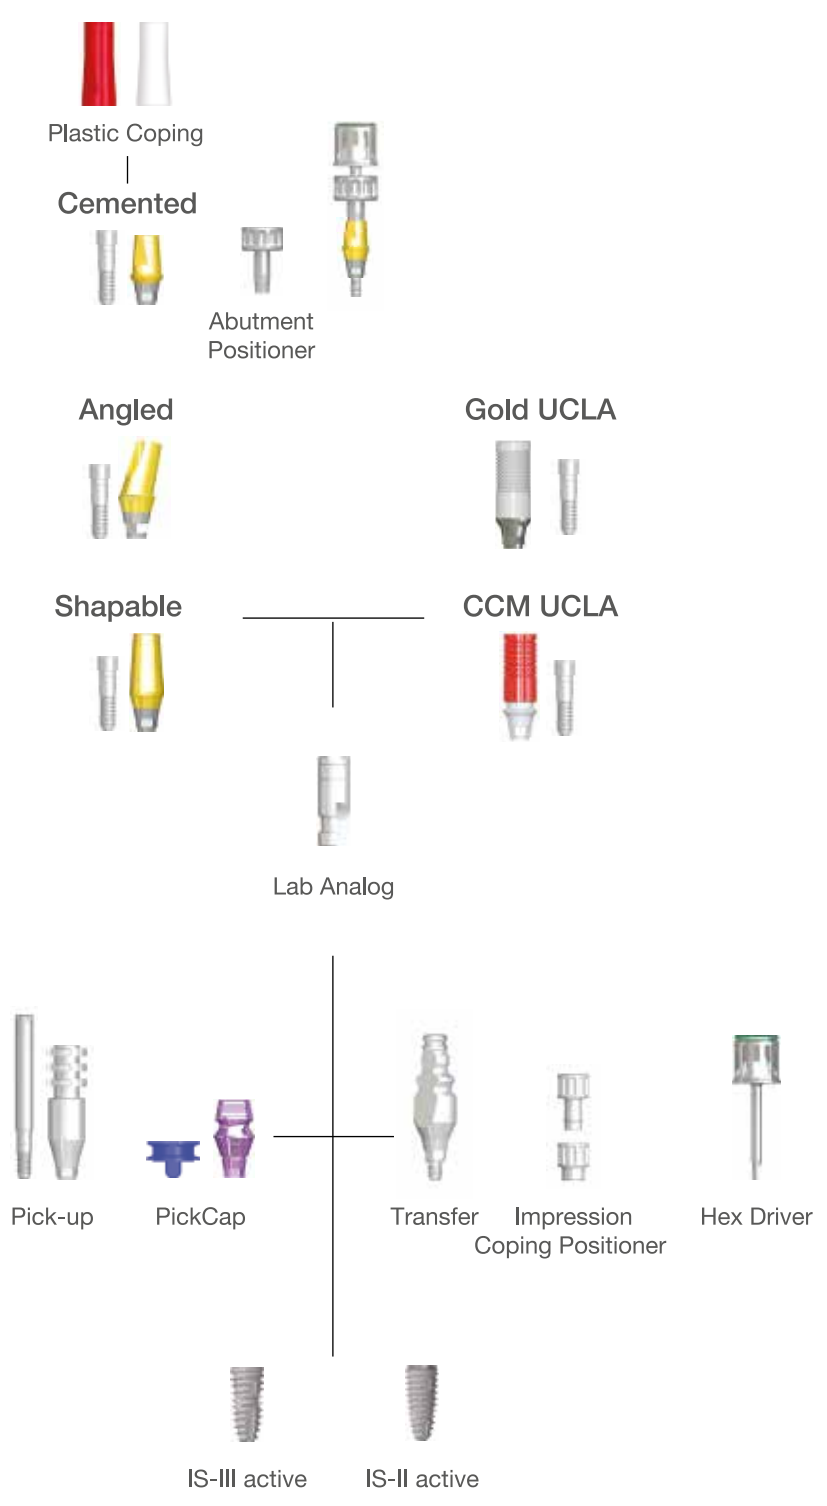



Note. When abutments are connected to Narrow Fixture(Ø3.5) or Short Fixture(7.3mm), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-II active)

When abutments are connected to Narrow Fixture(Ø3.5), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-III active)

IS Transfer Impression Coping



• Diameter Ø 4.8

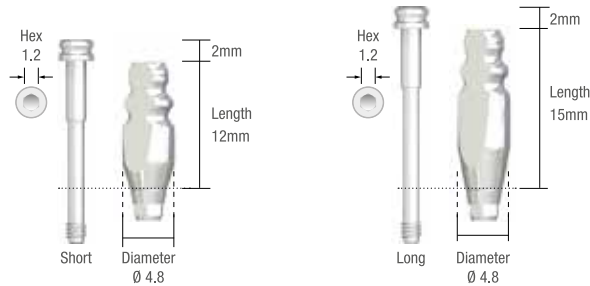Type	Hex	Non-Hex
Short	ISITH411	ISITN411
Long	ISITHL411	ISITNL411

* Impression coping Screw included (Short - ISTIS20, Long - ISTISL20)



• Diameter Ø 5.5

Type	Hex	Non-Hex
Short	ISITH511	ISITN511
Long	ISITHL511	ISITNL511

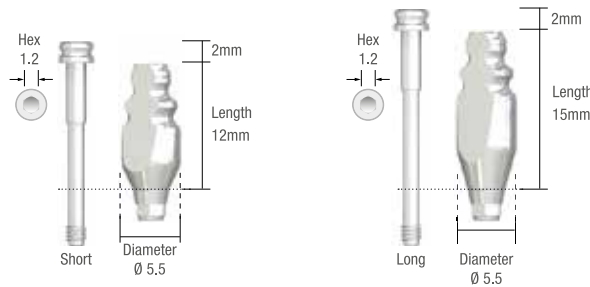* Impression coping Screw included (Short - ISTIS20, Long - ISTISL20)


• Diameter Ø 6.0

Type	Hex	Non-Hex
Short	ISITH611	ISITN611
Long	ISITHL611	ISITNL611

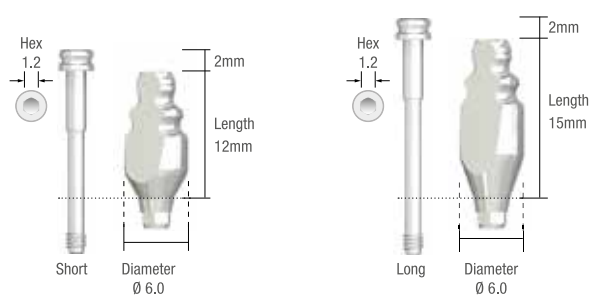* Impression coping Screw included (Short - ISTIS20, Long - ISTISL20)

• Impression Coping Hex Screw

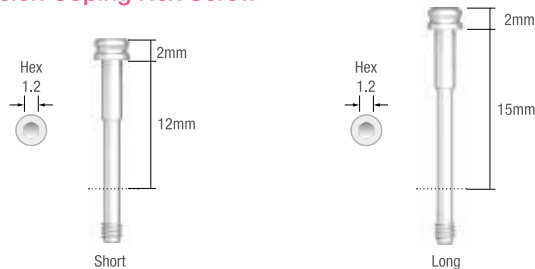

Short	ISTIS20H
Long	ISTISL20H

IS Transfer Impression Coping Positioner




Product name	FDHSET01
--------------	----------

* Connected to transfer impression coping

IS Pick-up Impression Coping


• Diameter $\varnothing 4.0$

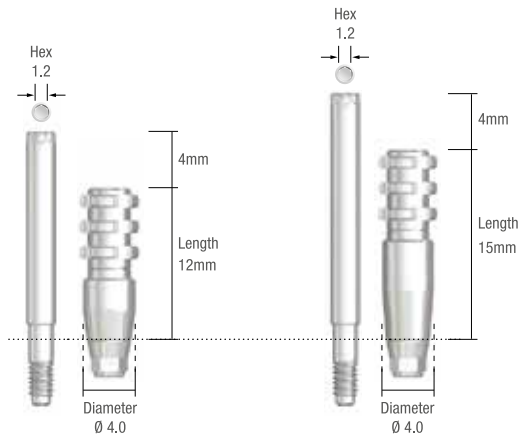

Type	Hex	SCRP®	Non-Hex
Short	ISIPH400	ISIPS400	ISIPN400
Long	ISIPHL400	ISIPSL400	ISIPNL400

* Impression coping Screw included
(Medium - ISPIS20)


• Diameter $\varnothing 4.5$

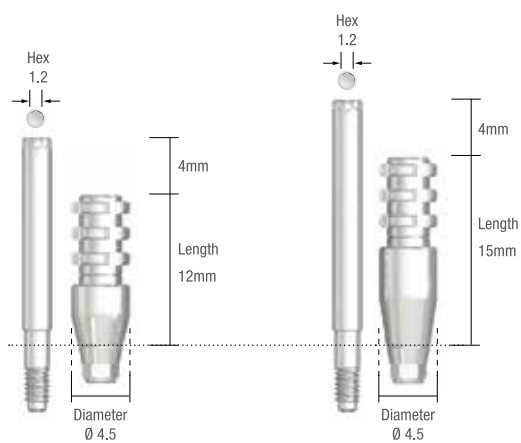

Type	Hex	SCRP®	Non-Hex
Short	ISIPH450	ISIPS450	ISIPN450
Long	ISIPHL450	ISIPSL450	ISIPNL450

* Impression coping Screw included
(Medium - ISPIS20)

• Diameter $\varnothing 4.8$

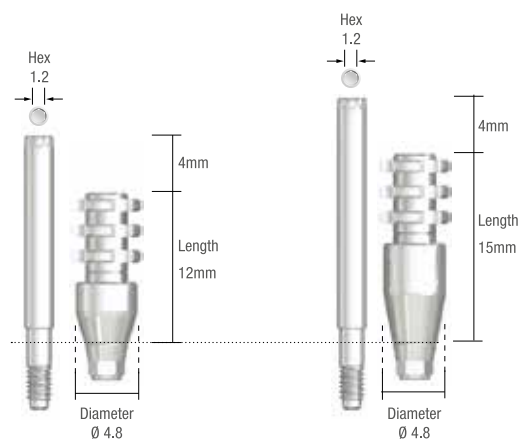


Type	Hex	SCRP®	Non-Hex
Short	ISIPH411	ISIPS411	ISIPN411
Long	ISIPHL411	ISIPSL411	ISIPNL411

* Impression coping Screw included
(Medium - ISPIS20, Long - ISPISL20)

IS Pick-up Impression Coping


• Diameter Ø 5.5

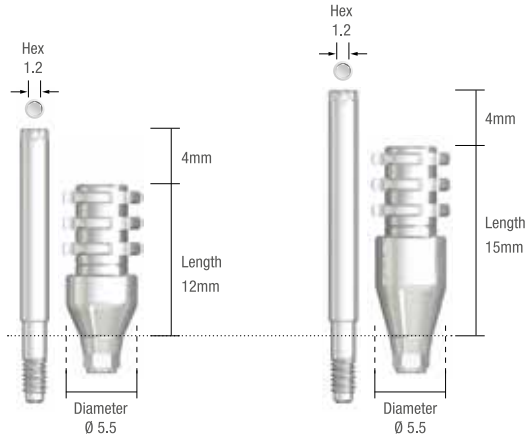

Type	Hex	SCRIP®	Non-Hex
Short	ISIPH511	ISIPS511	ISIPN511
Long	ISIPHL511	ISIPSL511	ISIPNL511

* Impression coping Screw included (Medium - ISPIS20, Long - ISPISL20)


• Diameter Ø 6.0

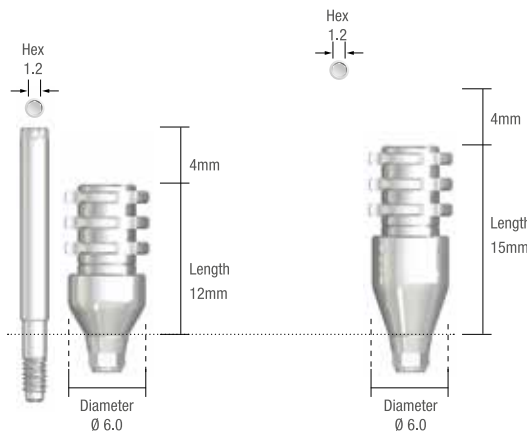


Type	Hex	SCRIP®	Non-Hex
Medium	ISIPH611	ISIPS611	ISIPN611
Long	ISIPHL611	ISIPSL611	ISIPNL611

* Impression coping Screw included (Medium - ISPIS20, Long - ISPISL20)

• Impression Coping Screw



X-Long	ISPIS20L
--------	----------

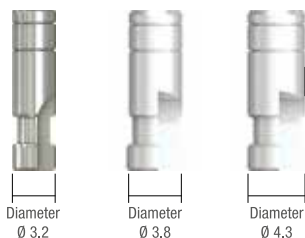

- * ISLA300 : S-Narrow (Ø3.2)
- * ISLA400 : Narrow (Ø3.5), All 7.3mm Fixtures
- * ISLA500 : Regular, Wide Fixture

IS Lab Analog




Diameter	3.2	3.8	4.3
Product name	ISLA300	ISLA400	ISLA500

IS Temporary Abutment

Customizable titanium abutment for temporary crown and bridges

- Abutment Screw (ISCS20) included, Tightening torque : 30 Ncm




Hex Type



Diameter	Ø 3.2	Ø 4.5		
Cuff	1.0	2.0	2.0	1.5
Length (mm)	11.5	6.0	8.0	13.0
Product name	ISAHT300 *	ISAHT460	ISAHT480	ISAHT4130

* This component is only for S-narrow fixture.


* ISCS16S : S-Narrow(Ø3.2)



SCRP® Type



Diameter	Ø 4.5		
Cuff	2.0	2.0	-
Length (mm)	6.0	8.0	13.0
Product name	ISAST460	ISAST480	ISAST4130



Non-Hex Type



Diameter	Ø 3.2	Ø 4.5			
Cuff	1.0	2.0	2.0	1.5	
Length (mm)	11.5	6.0	8.0	13.0	
Product name	Ø 4.5	ISANT300 *	ISANT460	ISANT480	ISANT4130

* This component is only for S-narrow fixture.

* ISCS16S : S-Narrow (Ø3.2)


IS Cemented Abutment (Hex Type)

Cementable or Screw-retained abutment for single tooth and bridges

- Customizable by grinding (need to remain at least 3mm of abutment length above fixture platform)
- Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm




• Diameter Ø 3.5



Cuff	3.0	4.0	5.0	7.0
Length (mm)	7.0 mm			
Product name	ISAH3537 *	ISAH3547 *	ISAH3557 *	ISAH3577 *


* These components are only for S-narrow fixture.
* ISCS16S : S-Narrow(Ø3.2)

• Diameter Ø 4.5



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAH4140	ISAH4240	ISAH4340	ISAH4440	ISAH4540
	5.5	ISAH415	ISAH425	ISAH435	ISAH445	ISAH455
	7.0	ISAH417	ISAH427	ISAH437	ISAH447	ISAH457

• Diameter Ø 5.2




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAH5140	ISAH5240	ISAH5340	ISAH5440	ISAH5540
	5.5	ISAH515	ISAH525	ISAH535	ISAH545	ISAH555
	7.0	ISAH517	ISAH527	ISAH537	ISAH547	ISAH557

• Diameter Ø 5.7



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAH6140	ISAH6240	ISAH6340	ISAH6440	ISAH6540
	5.5	ISAH615	ISAH625	ISAH635	ISAH645	ISAH655
	7.0	ISAH617	ISAH627	ISAH637	ISAH647	ISAH657

• Diameter Ø 6.5




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAH7140	ISAH7240	ISAH7340	ISAH7440	ISAH7540
	5.5	ISAH715	ISAH725	ISAH735	ISAH745	ISAH755

IS Cemented Abutment (SCR^P® Type)

Abutment for screw-cement retained prosthesis

- Short hex design, Retrievable within 20° between implants
- Customizable by grinding (need to remain at least 3mm of abutment length above fixture platform)
- Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm

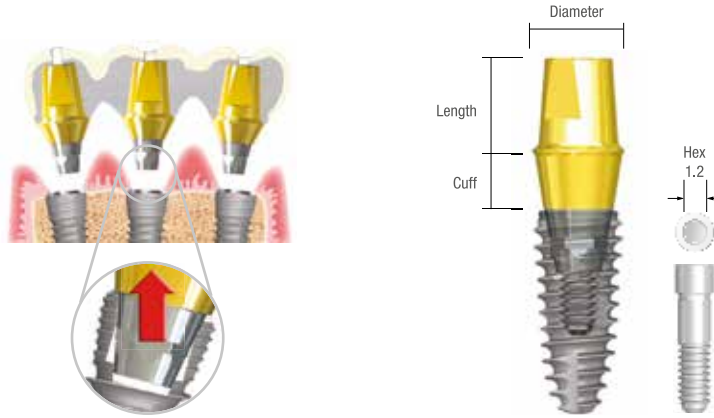


• Diameter Ø 4.5




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAS4140	ISAS4240	ISAS4340	ISAS4440	ISAS4540
	5.5	ISAS415	ISAS425	ISAS435	ISAS445	ISAS455
	7.0	ISAS417	ISAS427	ISAS437	ISAS447	ISAS457

• Diameter Ø 5.2



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAS5140	ISAS5240	ISAS5340	ISAS5440	ISAS5540
	5.5	ISAS515	ISAS525	ISAS535	ISAS545	ISAS555
	7.0	ISAS517	ISAS527	ISAS537	ISAS547	ISAS557

• Diameter Ø 5.7



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAS6140	ISAS6240	ISAS6340	ISAS6440	ISAS6540
	5.5	ISAS615	ISAS625	ISAS635	ISAS645	ISAS655
	7.0	ISAS617	ISAS627	ISAS637	ISAS647	ISAS657

• Diameter Ø 6.5



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAS7140	ISAS7240	ISAS7340	ISAS7440	ISAS7540
	5.5	ISAS715	ISAS725	ISAS735	ISAS745	ISAS755
	7.0	ISAS717	ISAS727	ISAS737	ISAS747	ISAS757

IS Cemented Abutment (Non-Hex Type)

Cementable or Screw-retained abutment for multiple or bridges

- Customizable by grinding (need to remain at least 3mm of abutment length above fi xture platform)
- Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm



• Diameter Ø 3.5




Cuff	3.0	4.0	5.0	7.0
Length	7.0 mm			
Product name	ISAN3537 *	ISAN3547 *	ISAN3557 *	ISAN3577 *

* These components are only for S-narrow fixture.


* ISCS16S : S-Narrow(Ø3.2)

• Diameter Ø 4.5




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAN4140	ISAN4240	ISAN4340	ISAN4440	ISAN4540
	5.5	ISAN415	ISAN425	ISAN435	ISAN445	ISAN455
	7.0	ISAN417	ISAN427	ISAN437	ISAN447	ISAN457

• Diameter Ø 5.2




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAN5140	ISAN5240	ISAN5340	ISAN5440	ISAN5540
	5.5	ISAN515	ISAN525	ISAN535	ISAN545	ISAN555
	7.0	ISAN517	ISAN527	ISAN537	ISAN547	ISAN557

• Diameter Ø 5.7



Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAN6140	ISAN6240	ISAN6340	ISAN6440	ISAN6540
	5.5	ISAN615	ISAN625	ISAN635	ISAN645	ISAN655
	7.0	ISAN617	ISAN627	ISAN637	ISAN647	ISAN657

• Diameter Ø 6.5




Cuff (mm)	1.0	2.0	3.0	4.0	5.0	
Length	4.0	ISAN7140	ISAN7240	ISAN7340	ISAN7440	ISAN7540
	5.5	ISAN715	ISAN725	ISAN735	ISAN745	ISAN755

IS Shapable Abutment


Customizable by grinding (need to remain at least 3mm of abutment length above fixture platform)

• Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm

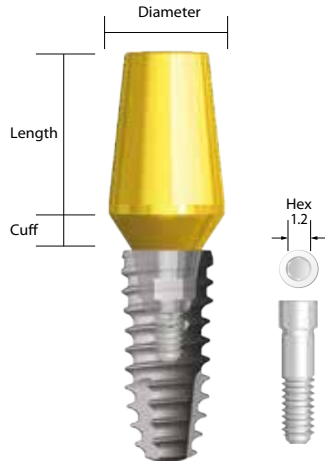


Narrow / Regular / Wide / S-wide

• Diameter $\varnothing 4.5$

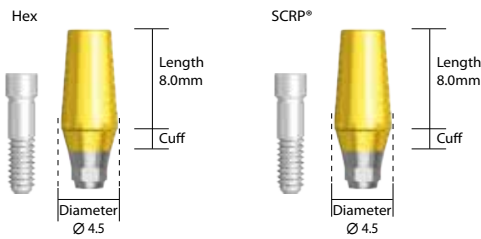


Cuff(mm)	2.0	4.0
Hex	ISSH428	ISSH448

• Diameter $\varnothing 5.2$

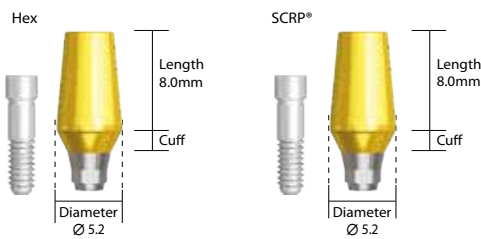


Cuff(mm)	2.0	4.0
Hex	ISSH528	ISSH548

• Diameter $\varnothing 5.7$

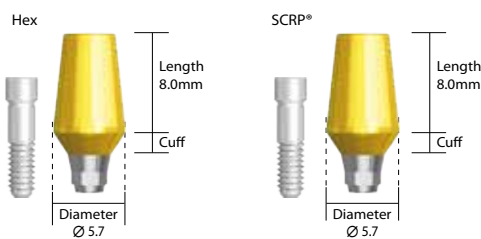

Cuff(mm)	2.0	4.0
Hex	ISSH628	ISSH648

• Diameter $\varnothing 6.5$

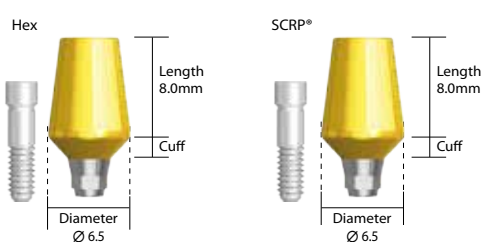

Cuff(mm)	2.0	4.0
Hex	ISSH728	ISSH748

IS 15° Angled Abutment

Customizable by grinding.

• Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm


A-Type

(Angle to the edge)



B-Type

(Angle to the flat wall)

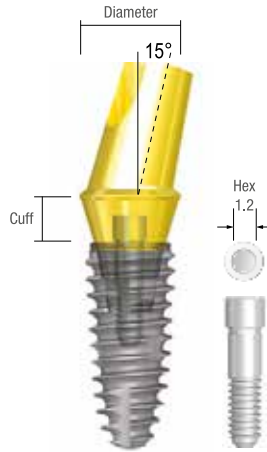

• Diameter Ø 3.2




Type	
Cuff (mm)	3.0
A Type	ISAHA1739
B Type	ISAHB1739

* These components are only for S-narrow fixture.

• Diameter Ø 4.5

A-Type

(Angle to the edge)




B-Type

(Angle to the flat wall)



Non-Hex




Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA1427	ISAHA1437	ISAHA1447
B Type	ISAHB1427	ISAHB1437	ISAHB1447
Non-Hex	ISANA1427	ISANA1437	ISANA1447

• Diameter Ø 5.2


A-Type

(Angle to the edge)




B-Type

(Angle to the flat wall)



Non-Hex




Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA1527	ISAHA1537	ISAHA1547
B Type	ISAHB1527	ISAHB1527	ISAHB1527
Non-Hex	ISANA1527	ISANA1537	ISANA1547

• Diameter Ø 5.7


A-Type

(Angle to the edge)




B-Type

(Angle to the flat wall)



Non-Hex



Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA1627	ISAHA1637	ISAHA1647
B Type	ISAHB1627	ISAHB1637	ISAHB1647
Non-Hex	ISANA1627	ISANA1637	ISANA1647

IS 25° Angled Abutment

Customizable by grinding. Can be positioned in 12 directions by selecting A or B type


• Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm

A-Type

(Angle to the edge)

B-Type


(Angle to the flat wall)

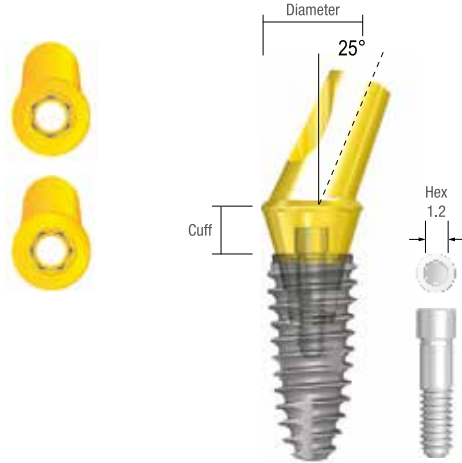

• Diameter Ø 4.5

A-Type

(Angle to the edge)



B-Type

(Angle to the flat wall)



Non-Hex



Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA2427	ISAHA2437	ISAHA2447
B Type	ISAHB2427	ISAHB2437	ISAHB2447
Non-Hex	ISANA2427	ISANA2437	ISANA2447

• Diameter Ø 5.2

A-Type

(Angle to the edge)




B-Type

(Angle to the flat wall)



Non-Hex




Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA2527	ISAHA2537	ISAHA2547
B Type	ISAHB2527	ISAHB2537	ISAHB2547
Non-Hex	ISANA2527	ISANA2537	ISANA2547

• Diameter Ø 5.7


A-Type

(Angle to the edge)




B-Type

(Angle to the flat wall)



Non-Hex





Cuff (mm)	2.0	3.0	4.0
A Type	ISAHA2627	ISAHA2637	ISAHA2647
B Type	ISAHB2627	ISAHB2637	ISAHB2647
Non-Hex	ISANA2627	ISANA2637	ISANA2647

IS CCM UCLA Abutment

Customizable by casting. Cementable or Screw-retained abutment for single tooth and bridges.


• Abutment Screw (ISCS20) included, Tightening Torque : 30 Ncm

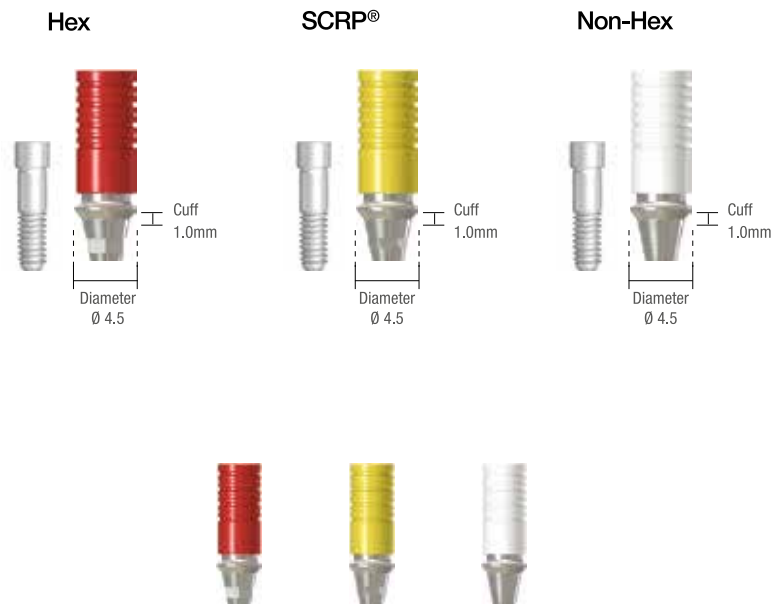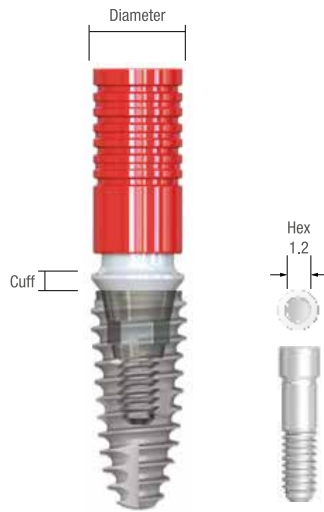

Hex	SCRP®	Non-Hex
ISUCH400	ISUCS400	ISUCN400

Prosthetic Flow Chart

- IS Multi Unit Abutment

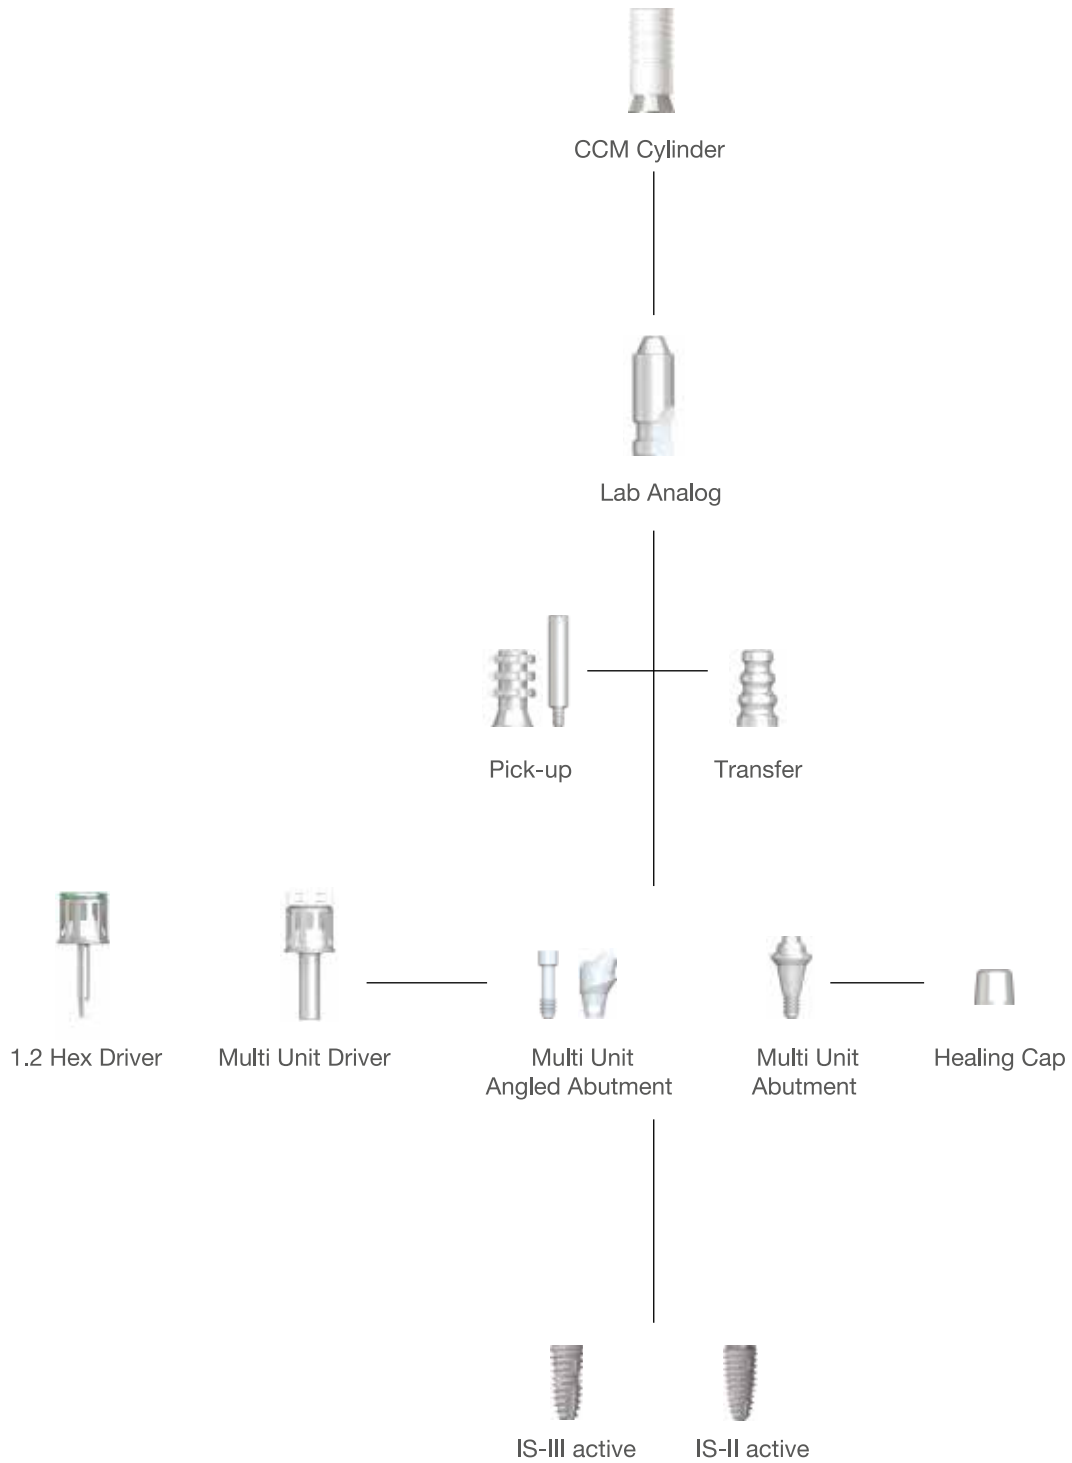

Note. When abutments are connected to Narrow Fixture(Ø3.5) or Short Fixture(7.3mm), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-II active)
 When abutments are connected to Narrow Fixture(Ø3.5), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-III active)


IS Multi Unit Abutment

Screw-retained abutment for multiple or bridges

• Abutment Tightening Torque : 30 Ncm, Cylinder screw 15 Ncm



Multi Unit Abutment



Cuff (mm)	1.0	2.0	3.0	4.0
Product name	ISMUA4810	ISMUA4820	ISMUA4830	ISMUA4840

* Holder(MUAH48) Included


IS Multi Unit Angled Abutment

Screw-retained abutment for multiple or bridges

• Abutment Tightening Torque : 30 Ncm, Cylinder screw 15 Ncm




Multi Unit Angled Abutment

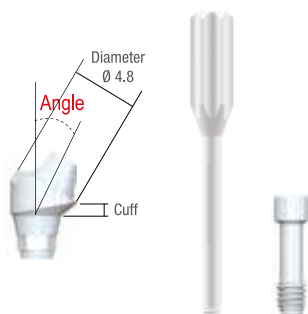

Cuff (mm)		1.0	2.0	3.0	4.0
Hex	17°	ISAHMUA1410S	ISAHMUA1420S	ISAHMUA1430S	ISAHMUA1440S
	30°	ISAHMUA3410S	ISAHMUA3420S	ISAHMUA3430S	ISAHMUA3440S
Non-Hex	17°	ISANMUA1410S	ISANMUA1420S	ISANMUA1430S	ISANMUA1440S
	30°	ISANMUA3410S	ISANMUA3420S	ISANMUA3430S	ISANMUA3440S

* Holder Included

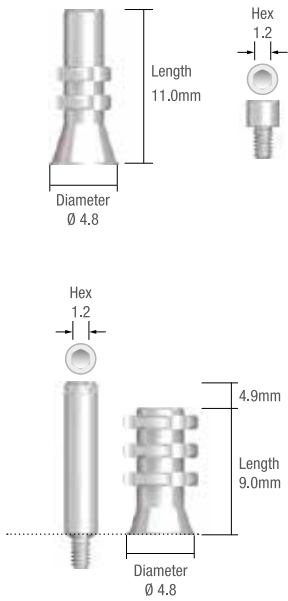


Temporary Cylinder, Non-Hex



Length(mm)	11.0
Product name	MUATPCN48


* Cylinder Screw(MUAS 14) Included

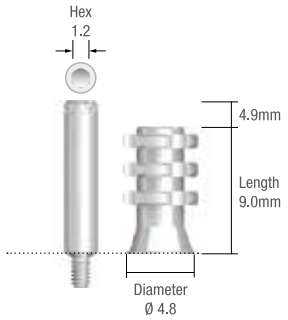

Pick-up Impression Copping



Length(mm)	9.0
Product name	MUAI48



Transfer Impression Copping




Length(mm)	9.0
Product name	MUAI48



Lab Analog



Product name	MUALA48
--------------	---------




CCM Cylinder, Non-Hex



Length(mm)	12.0
Product name	MUACCN48

* Cylinder Screw(MUAS 14) Included



Healing Cap



Length(mm)	4.1
Product name	MUAHC48

1.2 Hex Driver



Length (mm)	10mm	15mm
Product name	HD1210S	HD1215S


Multi Unit Abutment Driver



Product name	MUAD48S
--------------	---------

Prosthetic Flow Chart

- IS Ball Abutment

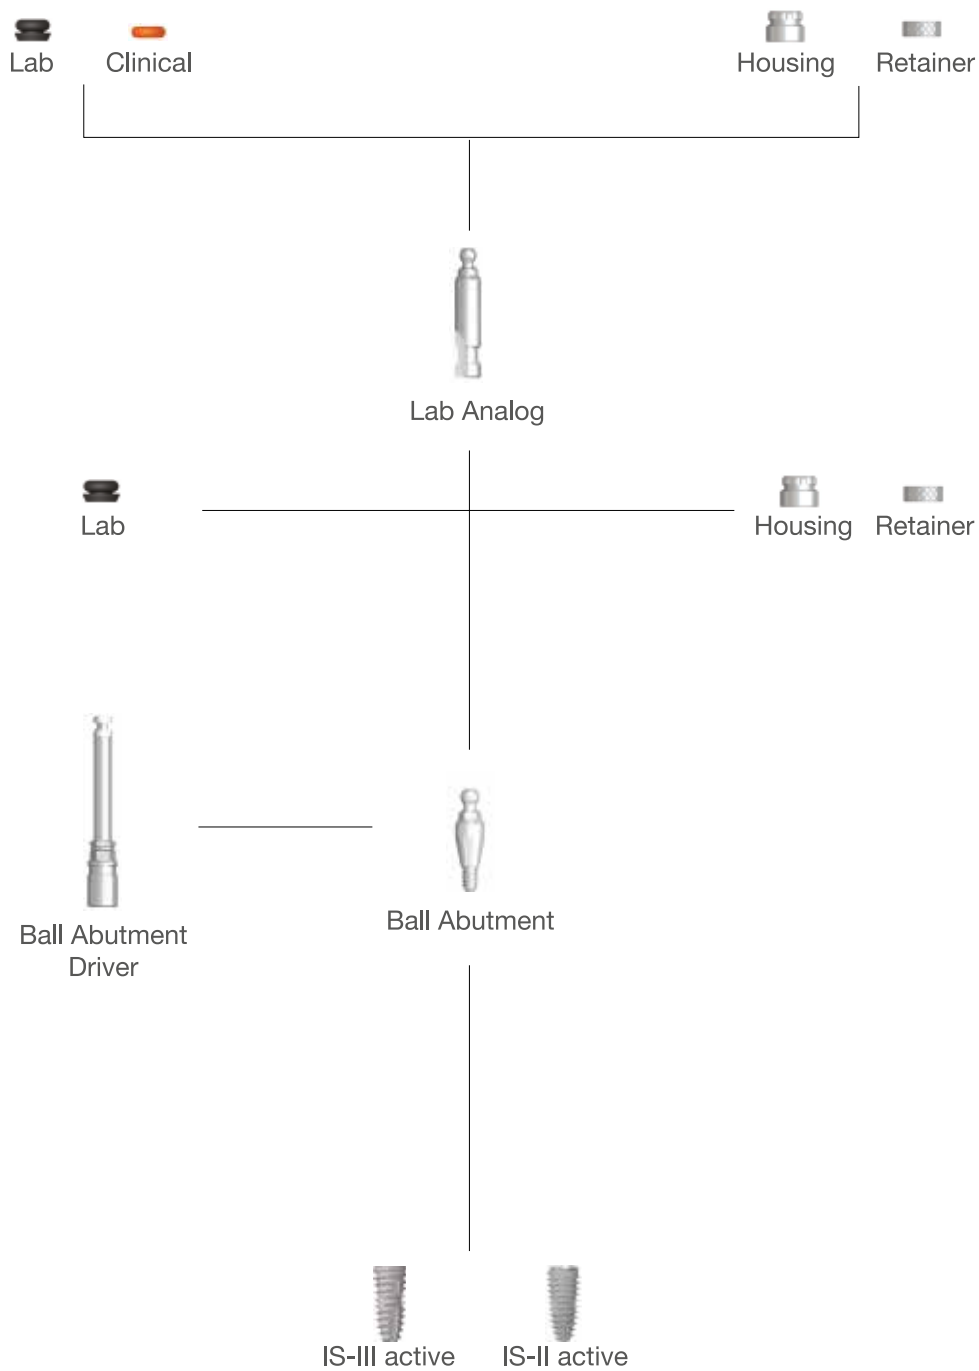

Note. When abutments are connected to Narrow Fixture($\varnothing 3.5$) or Short Fixture(7.3mm), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-II active)
 When abutments are connected to Narrow Fixture($\varnothing 3.5$), the total height of abutment is 0.4mm higher than Regular-Wide cases. (IS-III active)

IS Ball Abutment

Implant over-denture ball attachment system

- Compensation degree : Max 20° between implants
- Abutment Tightening Torque : 30 Ncm




Ball Abutment



Cuff (mm)	1.0	2.0	3.0	4.0
Product name	ISABA100	ISABA200	ISABA300	ISABA400

* Ball Abutment Driver(BADH24) Required


Housing



Product name	BAH40
--------------	-------

* O-ring(BAORING) 5ea and O-ring(BAOIMP) 1ea Included

Retainer



Product name	BAR20
--------------	-------

- * In case of occlusion interval is lower, use retainer instead of housing
- * O-ring(BAORING) 5ea and O-ring(BAOIMP) 1ea Included

IS Ball Abutment



O-Ring (Clinical)



Product name	BAORING
--------------	---------

* 3ea Included



O-Ring (Lab)



Product name	BAOIMP
--------------	--------

* 3ea Included

* Prevents the resin flowing into the under of Housing or Retainer


1. while making a final resin denture at laboratory.
2. while inserting Housing or Retainer within denture directly at the office.



Ball Lab Analog



Product name	BALA350
--------------	---------

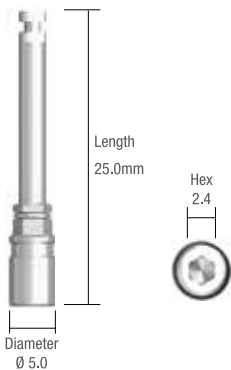

Ball Abutment Driver



Product name	BADH24
--------------	--------

Neobiotech **OT EQUATOR** Kit



Il Kit **Codice 130NBTx** include:

- 1 MONCONE IN TITANIO+TiN altezza a scelta (da 1 a 7mm)
- 1 CONTENITORE IN TITANIO ANODIZZATO viola
- 1 DISCHETTO PROTETTIVO
- 4 CAPPETTE RITENTIVE ASSORTITE (Gialla, Rosa, Bianca trasparente, Viola)




ACCESSORI E STRUMENTI

H (mm)
Altezza transmucosa



MONCONE **OT EQUATOR** in titanio nitrurato

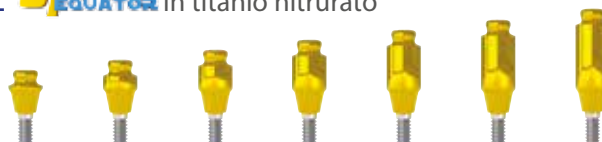

H (mm)	1	2	3	4	5	6	7
Codice	030NBT1	030NBT2	030NBT3	030NBT4	030NBT5	030NBT6	030NBT7

KIT DA LABORATORIO

Codice **192ECE**



Kit completo di accessori assortiti specifici per il laboratorio

Contiene

- 1 CONTENITORE in titanio 141CTE
- 1 CAPPETTA NERA 140CEN
- 1 DISCHETTO PROTETTIVO trasparente
- 4 CAPPETTE assortite
1 x Gialla 140CEG
1 x Rosa 140CER
1 x Bianca trasparente 140CET
1 x Viola 140CEV



CAPPETTA viola
(forte 2.700g)

Codice **140CEV**



CAPPETTA trasparente
(standard 1.800g)

Codice **140CET**



CAPPETTA nera
(per laboratorio)

Codice **140CEN**



CAPPETTA gialla
(extra-soft 600g)

Codice **140CEG**



CAPPETTA rosa
(soft 1.200g)

Codice **140CER**



CONTENITORE
cappette, titanio anodizzato viola

Codice **141CTE**



CONTENITORE
cappette, Inox

Codice **141CAE**



KIT SMART BOX
Auto-parallelizzante

Codice **335SBC**

Contiene

- 1 CONTENITORE SMARTBOX completo di cappetta nera da laboratorio
- 1 DISCHETTO PROTETTIVO rosa
- 4 CAPPETTE assortite (1 x tipo)



TRANSFER per impronta a strappo, con cappetta OT CAP normo

Codice **044CAIN**



CHIAVE A SEZIONE QUADRATA 1,25 mm comprensivo di HOLDER (cod. 774HC)

Codice **774CHE**

Per avvitare OT-Equator con cricchetto dinamometrico



ANALOGO da laboratorio

Codice **144AE**



ESTRATTORE/INSERITORE DI CAPPETTE RITENTIVE. Nei box metallici e nel cavo orale

Codice **485IC**

DIGITAL SOLUTIONS

Abutment Scan Body

Gli ScanBody permettono il preciso trasferimento della posizione degli impianti mediante scansione intraorale nello studio dentistico.

Grazie allo speciale design, sono in grado di trasferire posizioni 3D in modo estremamente preciso.

- Vite PSBSM20 compresa



1. ScanBody inserito sull'impianto



2. Ricezione dei dati digitali



3. Pianificazione dell'abutment



4. Abutment inserito sull'impianto



Diametro
Ø4.0
narrow (4)

Lungh.
17mm



Diametro
Ø5.0
regular (5)


Lungh.
14mm

Scan Body Hex Type



vite PSBSM20 inclusa

Multi Unit Abutment Scan Body





Diametro	4,8
Codice	MUASB48

vite MUASB 14 inclusa

Ti-Cylinder Abutment


Abutment in titanio per monconi customizzati.
 • Vite SCS20 compresa

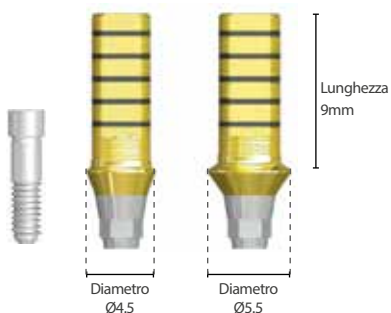

Type	Diametro	4.5	5.5
Hex	Codice	ISTCAH4509	ISTCAH5509
Non-Hex	Codice	ISTCAN4509	ISTCAN5509



Ti-Link Abutment



Type	Ø	4.0	4.5
Hex	Codice	ISLKH4035NB	ISLKH4535NB

Analoghi Digitali



Narrow



Regular/Wide




Diametro	Narrow	Regular/Wide
Codice	SGISLA400	SGISLA500


* SGISLA400 per impianti Narrow Ø3.5 e tutti gli impianti lung. 7.3
 SGISLA500 per impianti Regular e Wide

Surgical Guide Sleeve


Narrow




Regular/Wide



C-Sleeve Regular/Wide



Diametro	5,5	7	7
Distanza antirotazionale	4,1	5,2	5,2
Altezza	3,5	3,5	3,5
Codice	SGS55N	SGS70RW	CSGS70RW



Surgical Guide Fixed

Lateral pin



Lunghezza	18mm
Codice	SGLAP18L

Lateral sleeve



Diametro	3,0
Codice	SGLAS30L

Fresa per lateral pin



Codice	SGLAD15L
--------	----------

Avvitatori per lateral pin



Codice	SGCAC00
--------	---------

da contrangolo



Codice	SGRC10
--------	--------

da cricchetto




























NeoBiotech


IT IMPLANT SYSTEM

IT-III active

IT Implant System Chart

Fixture	Healing & Cover Screw	Abutment		Impression Coping	Lab Analog		
 IT-III active	 Healing Abutment  Cover Screw	Solid	Regular Neck	Solid 	 Impression Cap	 Regular Neck – Lab Analog (Abutment Level)	
				Excellent Solid		 Positioning Cylinder	 Shoulder Analog (Abutment Level)
			Wide Neck	Solid 	 Impression Cap  Positioning Cylinder	 Wide Neck – Lab Analog (Abutment Level)	
		Cemented			 Pick-up  Octa Non-Octa  Transfer  Octa Non-Octa  Transfer Impression Coping Positioner	 Regular Neck – Lab Analog (Fixture Level)  Wide Neck – Lab Analog (Fixture Level)	
		Angled		CCM  Octa Non-Octa			
		UCLA	Regular Neck	CCM (Wide Neck)  Octa Non-Octa			
			Wide Neck				


IT-III active

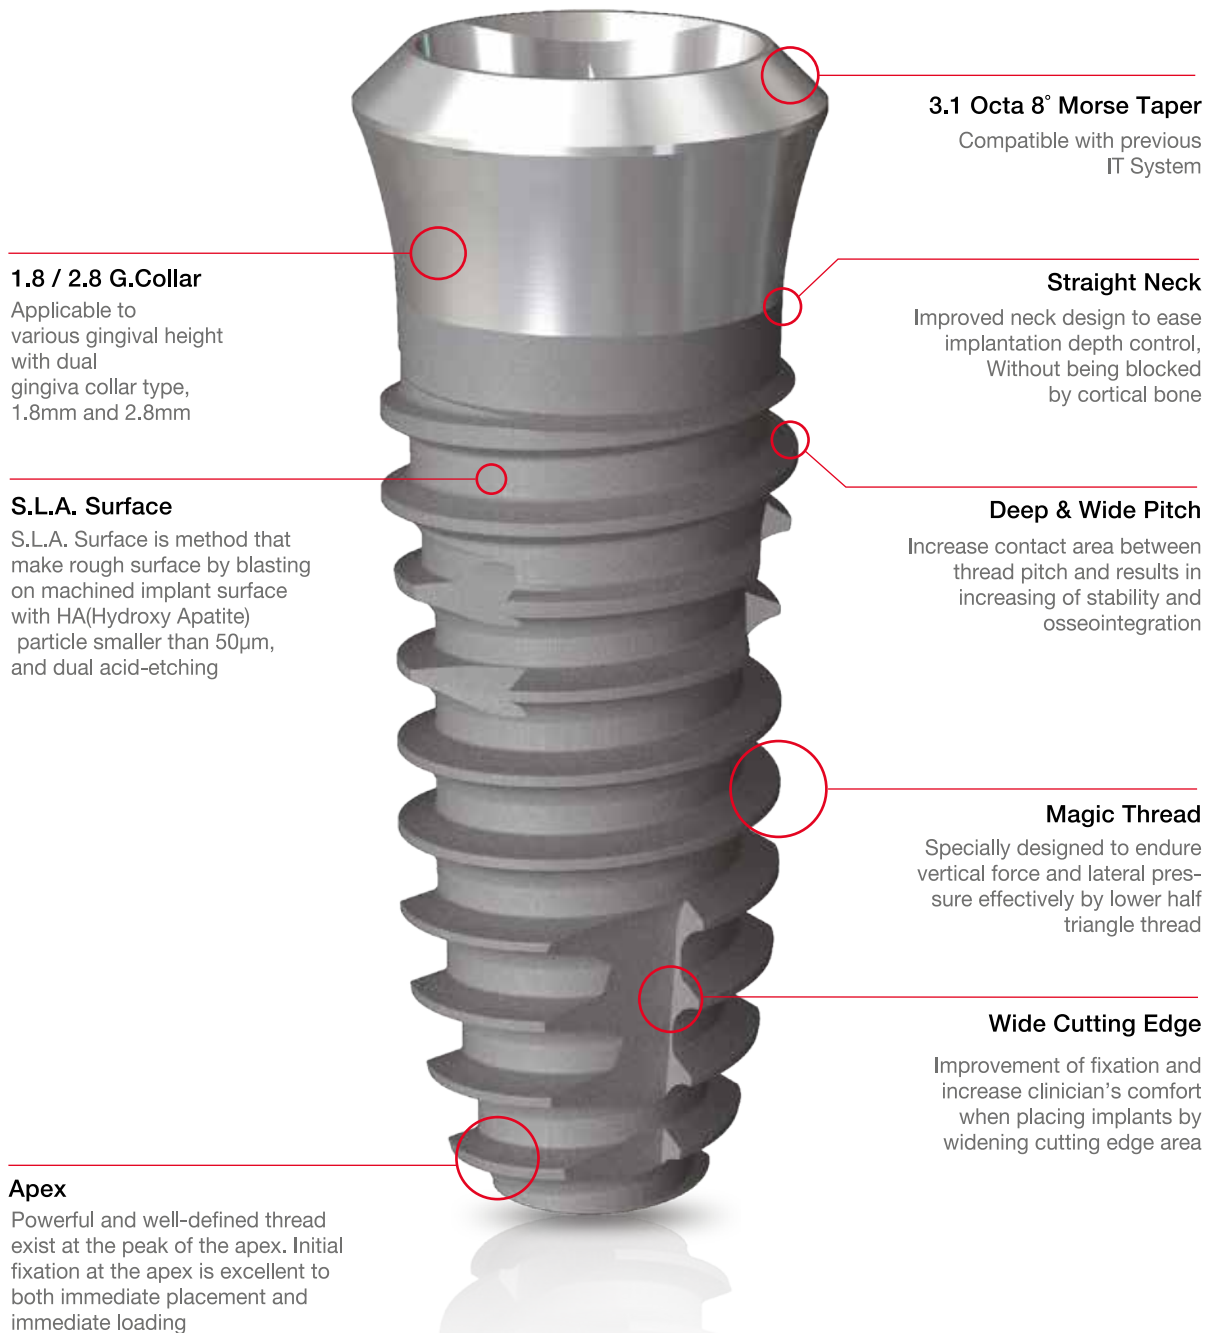

IT-III active Fixture (S.L.A. Surface)

The fixture bigger than Ø4.5 diameter is recommended to be placed in posterior area.


* Regular Neck



• Narrow / Diameter Ø 3.5 / G.Collar 1.8mm




Length (mm)	8.5	10.0	11.5	13.0
Product name	IT313508AP	IT313510AP	IT313511AP	IT313513AP



• Regular / Diameter Ø 4.0 / G.Collar 1.8mm




Length (mm)	7.0	8.5	10.0	11.5	13.0
Product name	IT314007AP	IT314008AP	IT314010AP	IT314011AP	IT314013AP



• Regular / Diameter Ø 4.5 / G.Collar 1.8mm



Length (mm)	7.0	8.5	10.0	11.5	13.0
Product name	IT314507AP	IT314508AP	IT314510AP	IT314511AP	IT314513AP



• Regular / Diameter Ø 5.0 / G.Collar 1.8mm




Length (mm)	7.0	8.5	10.0	11.5	13.0
Product name	IT315007AP	IT315008AP	IT315010AP	IT315011AP	IT315013AP

* All measurements can be different with the actual size


IT Healing Abutment

Temporary restorations for contouring of the soft tissue

Tightening Torque : 8~10 Ncm

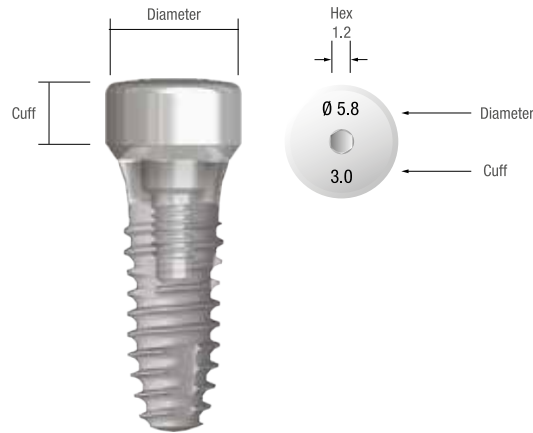

• Regular Neck





Diameter \varnothing 5.8



Cuff (mm)	2.0	3.0	4.0
Product name	IUTH502	IUTH503	IUTH504


Prosthetic Flow Chart

- IT Abutment



IT Transfer Impression Coping


• Regular Neck

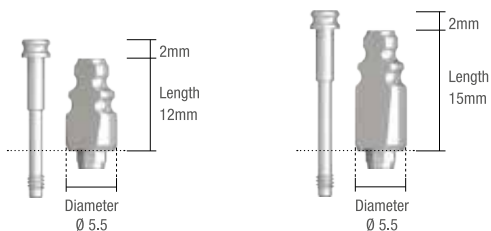

Type	Octa	Non-Octa
Short	ITIT0511	ITITN511
Long	ITITOL511	ITITNL511

* Impression Coping Screw Included (ITTIS20H)


• Impression Coping Hex Screw



Product name	ITTIS20H
--------------	----------

IT Transfer Impression Coping Positioner


* Connected to transfer impression coping



Product name	FDHSET01
--------------	----------

IT Pick-up Impression Coping

• Regular Neck

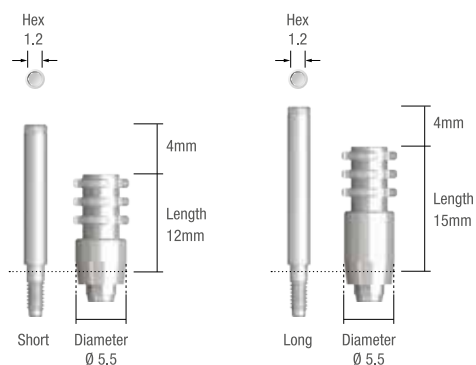

Type	Octa
Short	ITIP0511
Long	ITIPOL511

* Impression Coping Screw Included (Short : ITPIS20 / Long : ITPIS20L)

• Regular Neck



IT Lab Analog


Product name	ITLA50
--------------	--------

IT Cemented Abutment


IT SCRCP Abutment

Cementable or Screw-retained abutment for single tooth and bridges

- Semi-octa structure of SCRCP Abutment simplifies both installation and removal of prosthetic within 16 degrees in multiple cases
- Customizable by grinding (need to remain at least 3mm of abutment length above fixture platform)
- Abutment Screw(ITCS20S) included, Tightening Torque : 30Ncm

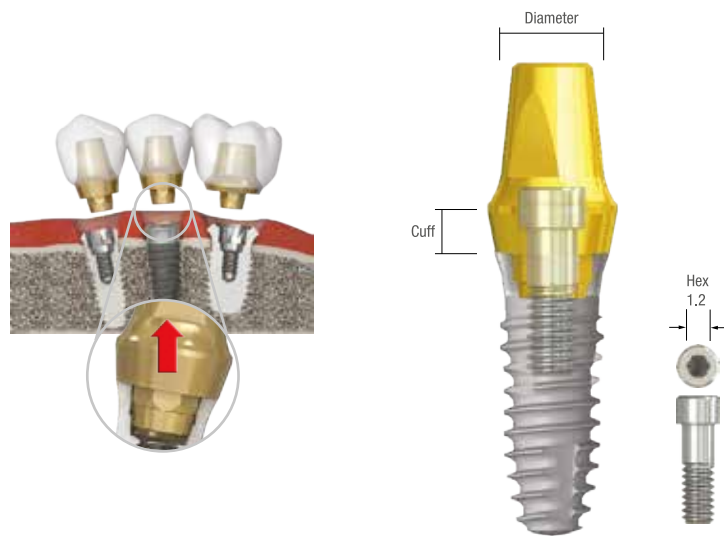

• Regular Neck

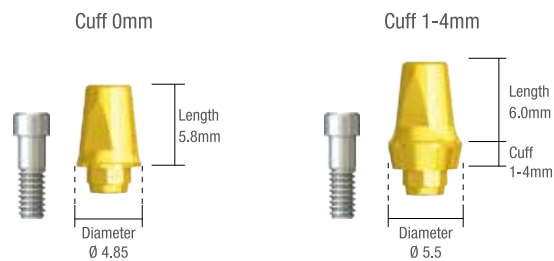

Diameter Ø5.5



Cuff (mm)	0	1.0	2.0	3.0	4.0
Octa	IC0500	IC0510	IC0520	IC0530	IC0540
Non-Octa	ICN500	ICN510	ICN520	ICN530	ICN540
SCRCP	ICS500	ICS510	ICS520	ICS530	ICS540

IT Pre Angled Abutment

• Abutment Screw(ITAS20S) included, Tightening Torque : 30 Ncm


A-Type

(Angle to the edge)



B-Type

(Angle to the flat wall)

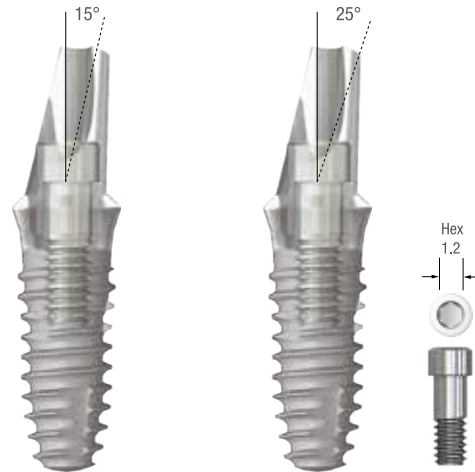

• Regular Neck



A - Type

Angle to the edge




B - Type

Angle to the flat wall

15°



Type	A	B
Product name	IA0310A	IA0310B



A - Type

Angle to the edge



B - Type

Angle to the flat wall

25°



Type	A	B
Product name	IA0320A	IA0320B


IT Collared Angled Abutment

• Abutment Screw(ITCS20S) included, Tightening Torque : 30 Ncm


A-Type
(Angle to the edge)



B-Type
(Angle to the flat wall)

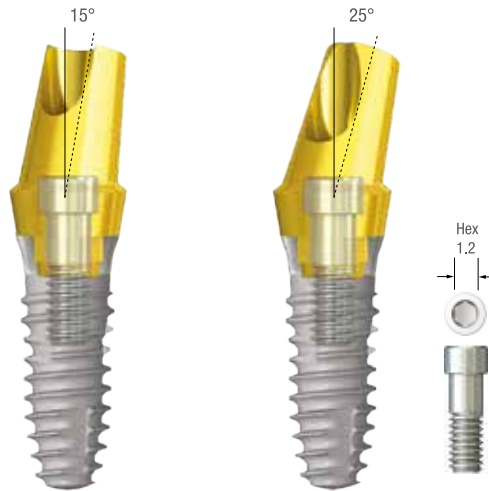


• Regular Neck

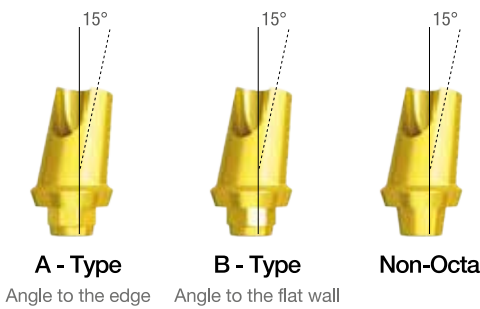

15°



Type	A		B		Non-Octa	
Cuff (mm)	1	2	1	2	1	2
Product name	IA0511A	IA0512A	IA0511B	IA0512B	IAN511	IAN512

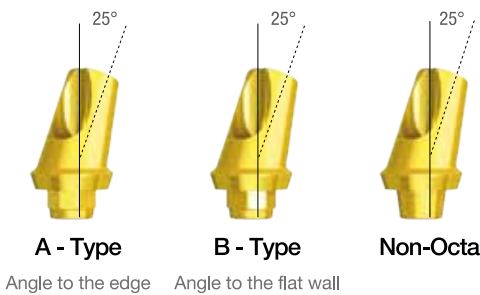

25°




Type	A		B		Non-Octa	
Cuff (mm)	1	2	1	2	1	2
Product name	IA0521A	IA0522A	IA0521B	IA0522B	IAN521	IAN522

IT CCM UCLA Abutment

Customizable by casting. Cementable or Screw-retained abutment for single tooth and bridges.

- Abutment Screw(ITCS20S) included, Tightening Torque : 30 Ncm
- Metal Casting

• Regular Neck



Diameter \varnothing 5.5



Type	Octa	Non-Octa
Product name	ITUC0500	ITUCN500


The image features three wireframe trays of surgical instruments, arranged in a descending staircase pattern from top-right to bottom-left. Each tray is filled with various surgical tools, including forceps, scalpels, and probes, all rendered in a white wireframe style against a dark background. The text is overlaid on the middle tray.

NeoBiotech

SURGICAL KIT
PROSTHETIC KIT


Neo Master Kit

This kit can be used to perform implant surgery for IS-III active, IS-II active, IT-III active

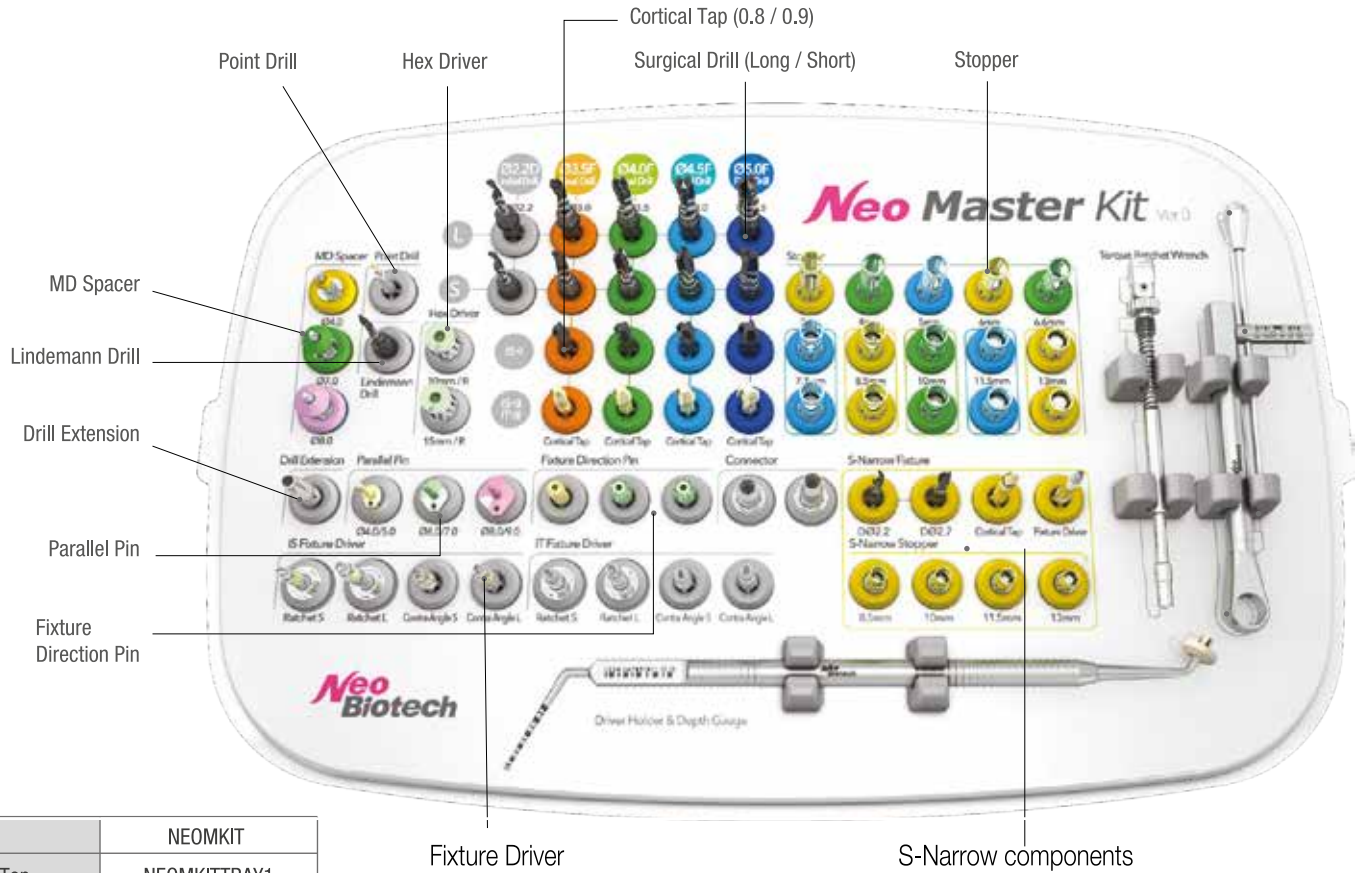


Kit	NEOMKIT
Kit Tray Top	NEOMKITTRAY1
Kit Tray Middle	NEOMKITTRAY2
Kit Tray Bottom	NEOMKITTRAY3

• Drill Length Guide

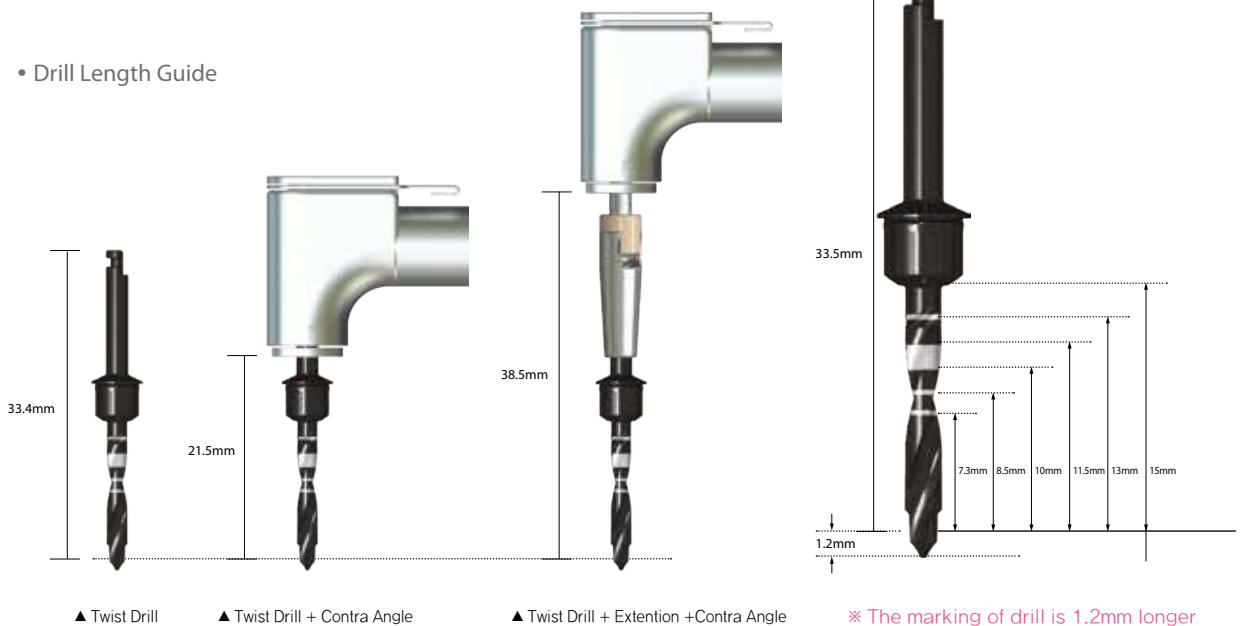


Neo Master Kit Components

• Point Drill

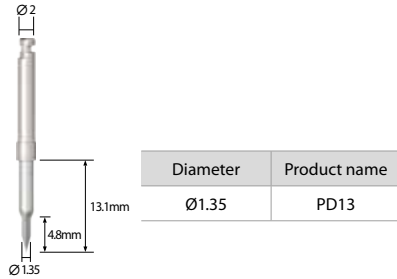

Diameter	Product name
Ø1.35	PD13


• Lindemann Drill

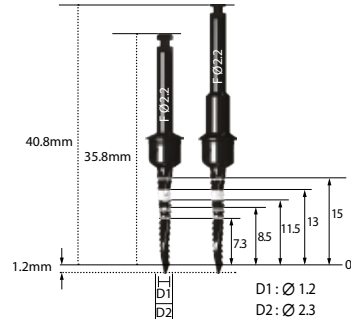

Diameter	Product name
Ø2.3	LDS23CS*
Ø2.3	LDS23CL*



* Optional

• Initial Drill

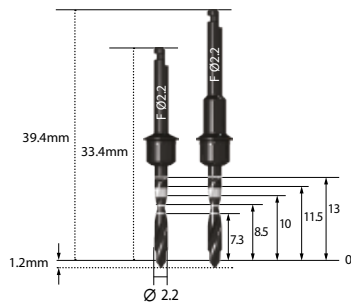

Diameter	Type	Product name
Ø2.2	Short	TSD22CS
Ø2.2	Long	TSD22CL

• Twist Drill

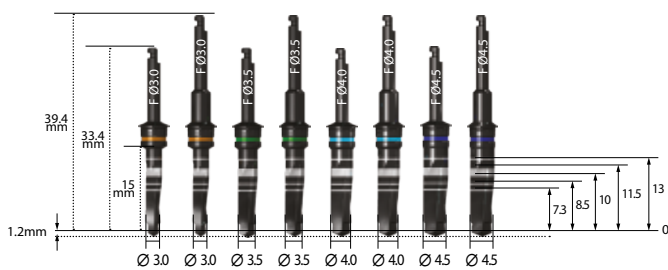

Diameter	Type	Product name
Ø3.0	Short	TSD30CS
Ø3.0	Long	TSD30CL
Ø3.5	Short	TSD35CS
Ø3.5	Long	TSD35CL
Ø4.0	Short	TSD40CS
Ø4.0	Long	TSD40CL
Ø4.5	Short	TSD45CS
Ø4.5	Long	TSD45CL

• Stopper


Stopper	3.0	4.0	5.0	6.0	6.6	7.3	8.5	10.0	11.5	13
Drilling Length(mm)	4.2*	5.2*	6.2*	7.2*	7.8	8.5	9.7	11.2	12.7	14.2
Product name	DS030C	DS040C	DS050C	DS060C	DS066C	DS070C	DS085C	DS100C	DS115C	DS130C



*Only Stopper included. Please order Stopper holder(DSHC) separately.
 * Not included, Separately Purchasable

Neo Master Kit Components

• Direction Pin



Diameter	Product name
Ø3.6	DP36
Ø4.5	DP45

• Cortical Drill



Diameter	Product name
Ø3.5	CD38*
Ø4.0	CD43*
Ø4.5	CD45*
Ø5.0	CD50*

* Optional

• EB Fixture Driver



Type	Hex	Product name
Narrow	2.4	EBFDH24*
Regular/Wide(3i)	2.7	EBFDH27*
Wide(Brenemark)	3.4	EBFDH34*


* Not Included.
Separately Purchasable.

• Drill Extension



Product name	DE01
--------------	------

• Hex Driver



Length(mm)	Hex	Product name
10	1.2	HD1210S
15		HD1215S
10	0.9	HD0910*
15		HD0910S*


* Not Included.
Separately Purchasable.

• Torque Ratchet



Product name	TW60
--------------	------


• Driver Holder & Depth Gauge

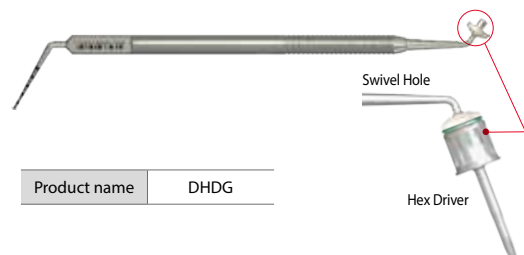

Product name	DHDG
--------------	------

Neo Master Kit Components

• Direction Pin



Diameter	Product name
Ø3.6	DP36
Ø4.5	DP45

• Cortical Drill



Diameter	Product name
Ø3.5	CD38*
Ø4.0	CD43*
Ø4.5	CD45*
Ø5.0	CD50*

* Optional

• EB Fixture Driver



Type	Hex	Product name
Narrow	2.4	EBFDH24*
Regular/Wide(3i)	2.7	EBFDH27*
Wide(Brenemark)	3.4	EBFDH34*


* Not Included.
Separately Purchasable.

• Drill Extension



Product name	DE01
--------------	------

• Hex Driver



Length(mm)	Hex	Product name
10	1.2	HD1210S
15		HD1215S
10	0.9	HD0910*
15		HD0910S*


* Not Included.
Separately Purchasable.

• Torque Ratchet



Product name	TW60
--------------	------

• Driver Holder & Depth Gauge

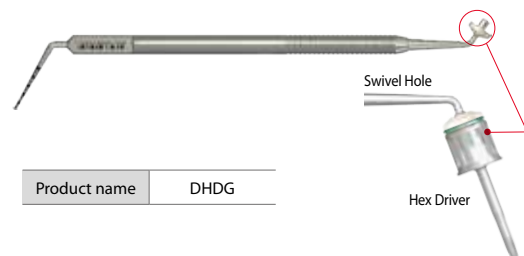

Product name	DHDG
--------------	------

Neo Master Kit Components


• S-Narrow Surgical Drill



Diameter	Product name
Ø2.2	TSDS22CL*
Ø2.7	TSD27CL*

* Not Included.
Separately Purchasable.

• S-Narrow Cortical Tap



Diameter	Product name
Ø3.2	CT32S09*

* Not Included.
Separately Purchasable.

• S-Narrow Drill Stopper



Length(mm)	8.5	10	11.5	13
Product name	DS085CS*	DS100CS*	DS115CS*	DS130CS*

* Please order Stopper holder(DSHCS) separately

* Not Included.
Separately Purchasable.

• S-Narrow Fixture Driver




Type	Product name
Contra Angle	ISFDSNCL*

* Not Included.
Separately Purchasable.


Neo Master Kit – Drilling Sequence

Drilling Speed & Torque


- Point Drill, Initial Drill, Twist Drill : 1,200rpm / 35~45Ncm
Cortical Tap : 50rpm / 50Ncm
- IS-III active(IT-III active) Fixture $\varnothing 4.0$ X 10mm (D1/D2 bone)

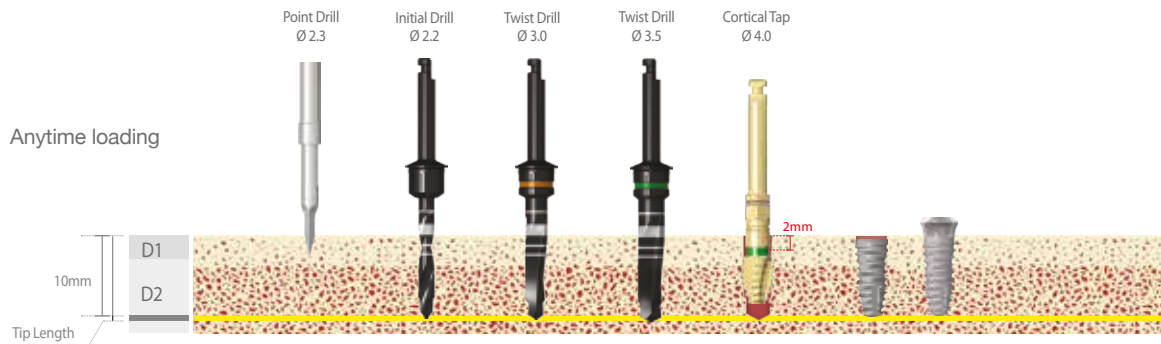

- IS-III active(IT-III active) Fixture $\varnothing 4.0$ X 10mm (D1/D2 bone)

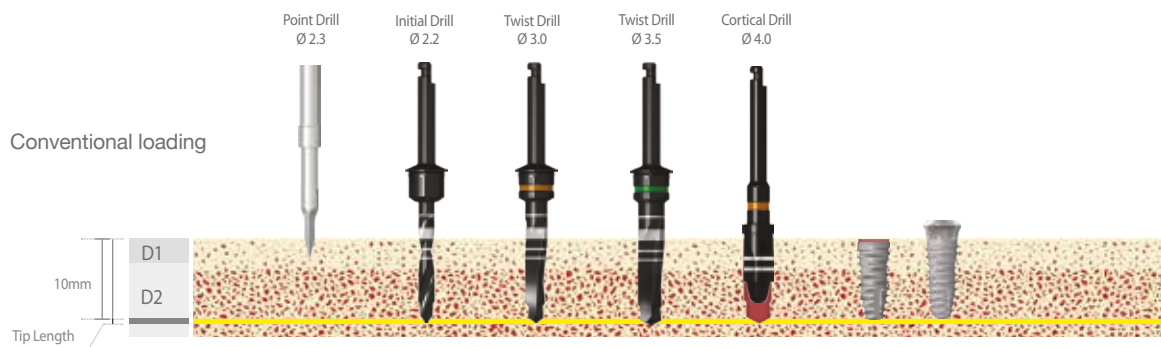


- IS-III active(IT-III active) Fixture $\varnothing 4.0$ X 10mm (D3/D4 bone)

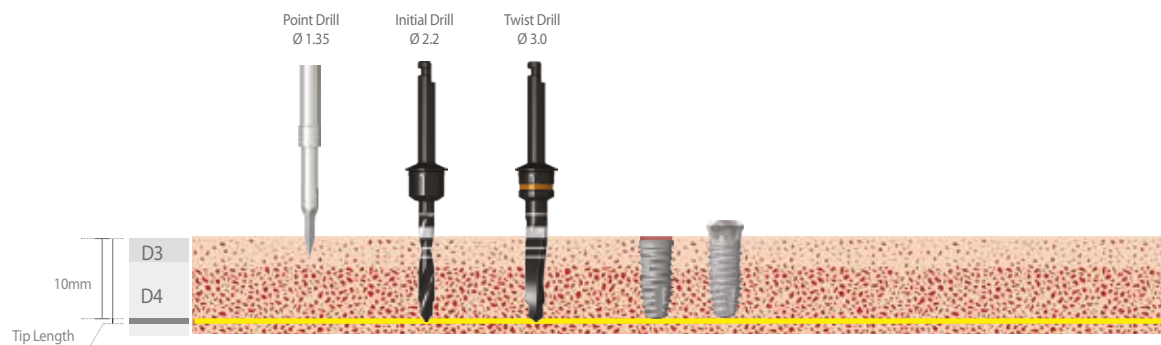

Neo NaviGuide Kit


This kit can be used to perform surgical guide implant surgery for IS-II active , IS-III active (Ø3.5~Ø5.0) For R/W sleeve , R/W C sleeve

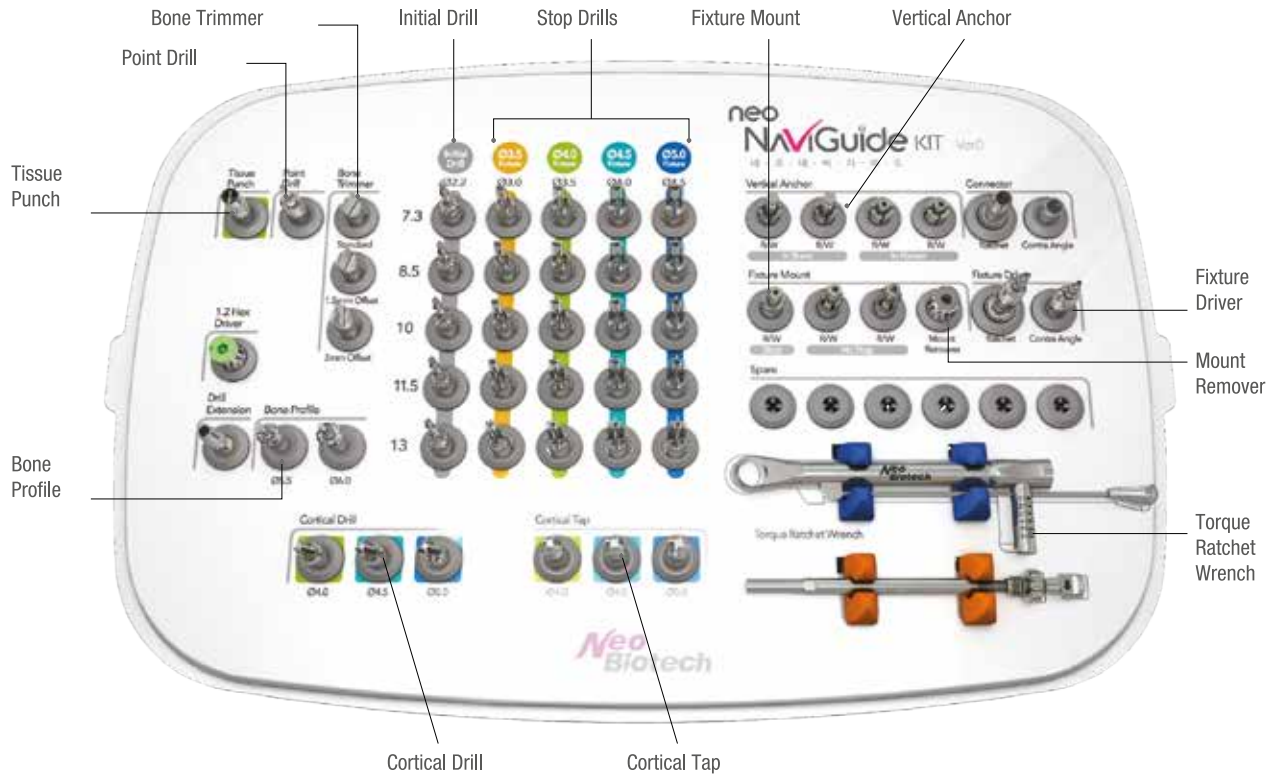


Product name	NEONGKIT
--------------	----------

Surgical Guide Sleeve


Narrow



Regular/Wide



C-Sleeve Regular/Wide




Diameter	5,5	7	7
Anti-rotational distance	4,1	5,2	5,2
Height	3,5	3,5	3,5
Product name	SGS55N	SGS70RW	CSGS70RW



Ridge Wider Kit


The product is a dental procedural device developed for convenient and easy split and expansion with RidgeWider Kit including expander, safe disk, drill and chisel in narrow ridge case where implant placement is difficult.

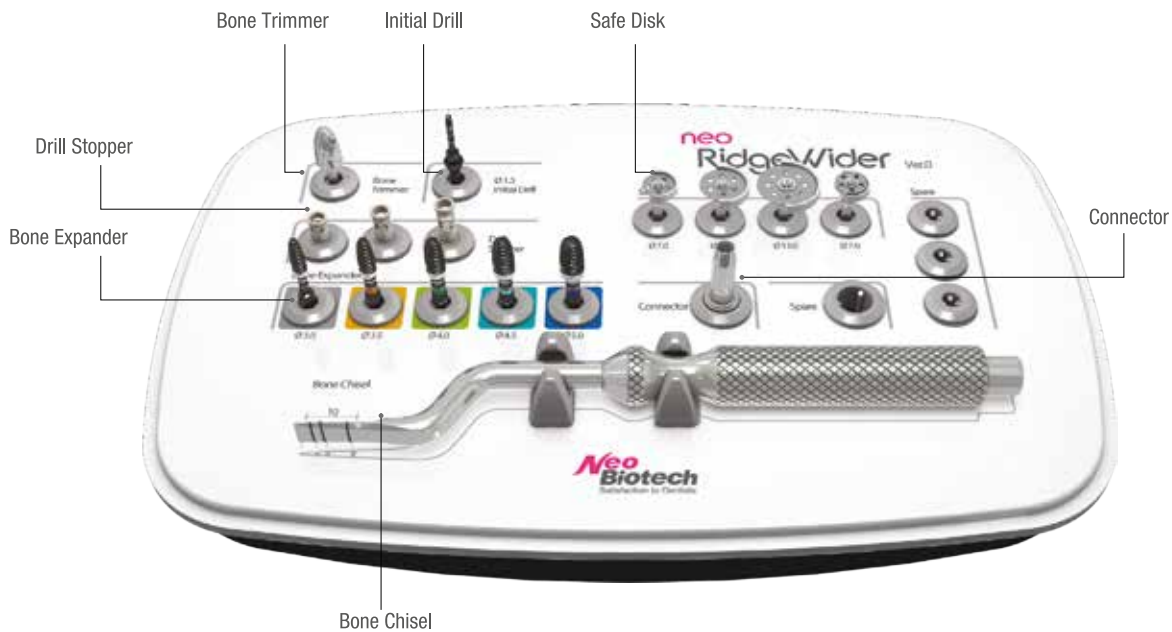

Kit

RWKIT


Neo Surgical Accessory Kit

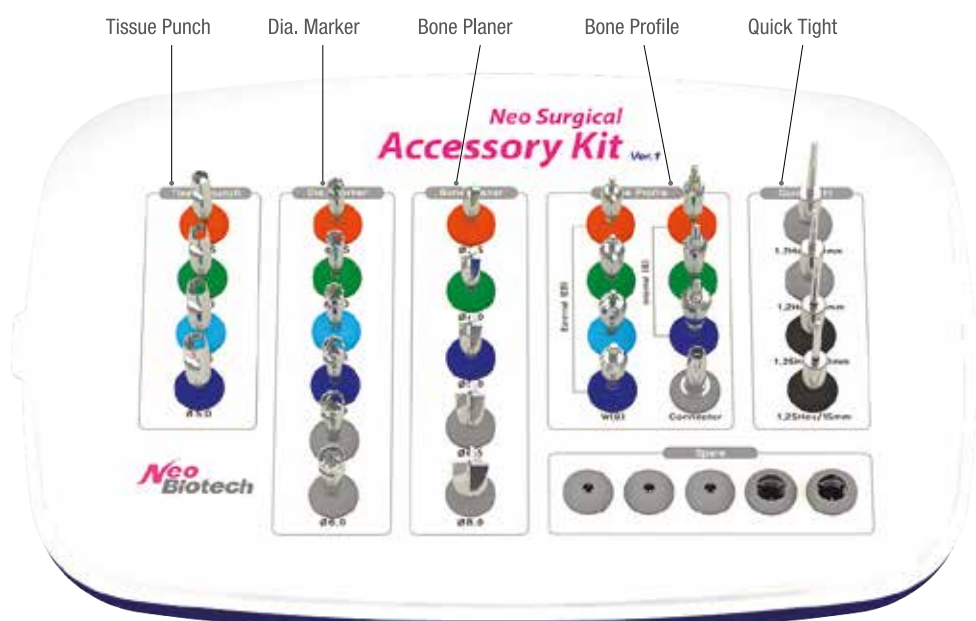

Kit

ACCKIT

Neo Prosthetic Kit

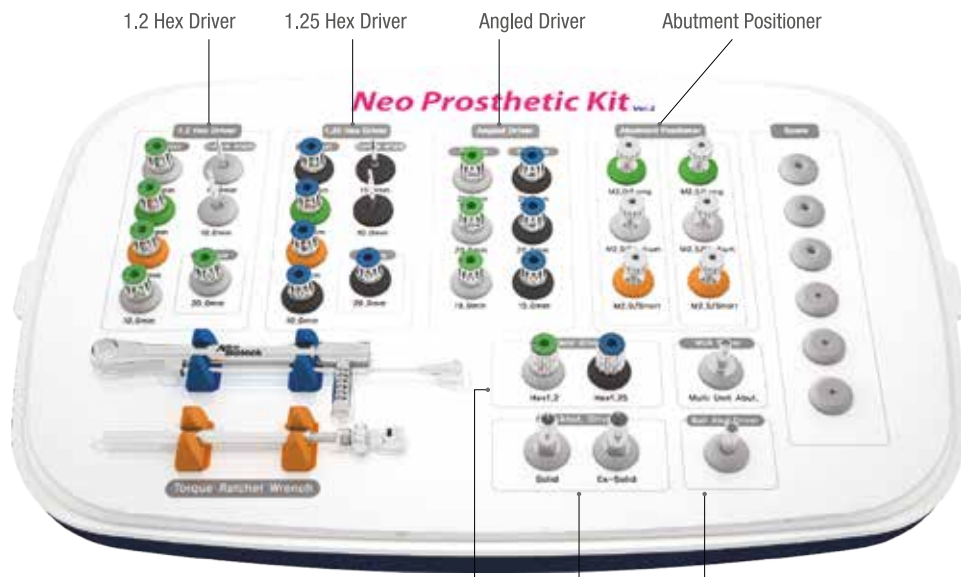

Kit PRTKIT

Hand Driver Extra Component


Neo Prosthetic Planning Kit

Neo Prosthetic Planning kit which helps users select a prosthesis by diameter, cuff and length when engaging with a fixture before choosing the size of prosthesis



Kit PRTPNKIT

• Hex Driver



Length (mm)	Hex	Product name
10	1.2	HD1210S
15		HD1215S

• Torque Ratchet




Product name TW60

The image features three wireframe 3D models of a Neobiotech Solution System. The top-left model shows a tray with a grid of wells, each containing a small cylindrical component, and a long, thin, curved tube. The bottom-left model shows a similar tray with a grid of wells, each containing a small cylindrical component, and a long, thin, curved tube with a textured, mesh-like section. The right-side model shows a tray with a grid of wells, each containing a small cylindrical component, and a long, thin, curved tube with a textured, mesh-like section. The text "Neobiotech SOLUTION SYSTEM" is centered in the middle of the image.

Neobiotech
SOLUTION SYSTEM


SCA Kit (Sinus Crestal Approach Kit)

SCA Kit is a drilling tool on the inferior cortical bone without tearing of membrane and make a perforation on the inferior cortical bone with out malleting osteotome technique Therefore User can get CMI Fixation. (Initial Fixation in Crest cortical bone, Middle cancellous bone and Inferior cortical bone)

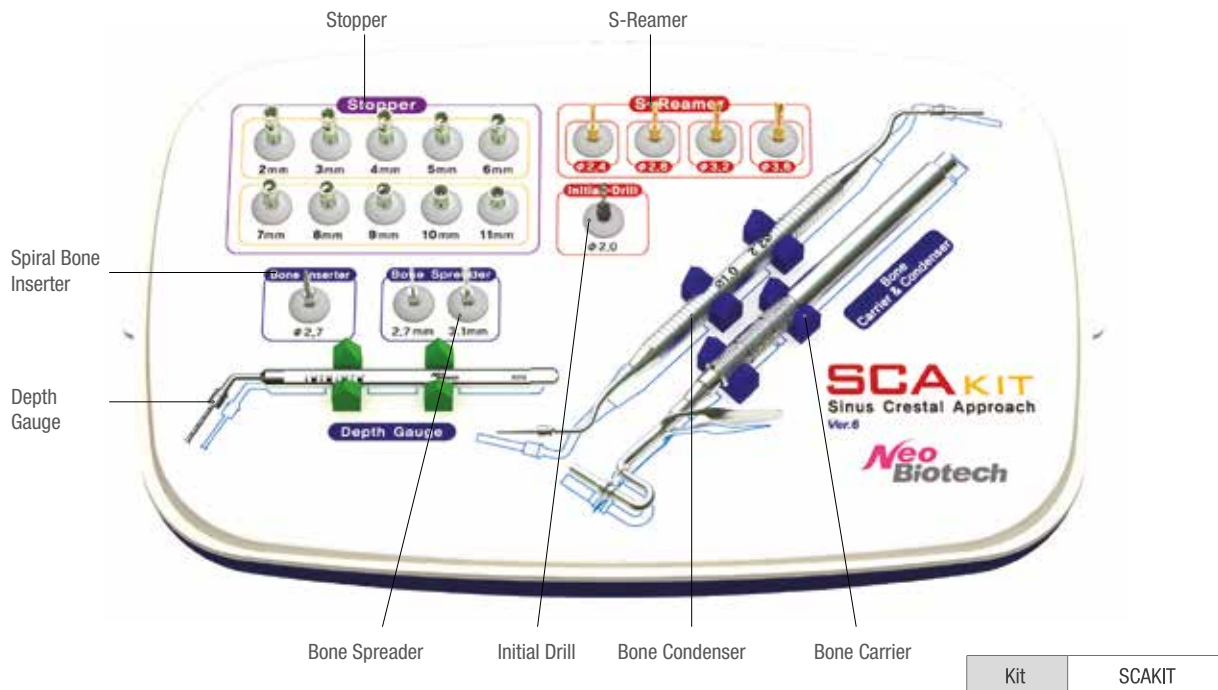

SLA Kit (Sinus Lateral Approach Kit)

Lateral window technique is the formation of the access to the maxillary sinus through its lateral wall. The process tool is simpler and much comfortable than any other techniques. Above all, this surgical kit provides ultimate solutions for the cases of only having with a thin residual bone height which is difficult to approach with a crestal technique, membrane rupture by a sinus crestal approach or placing a multiple implants. In addition, SLA reamers can be easily adapted for the case of formation of minimum flap size on the inferior wall.

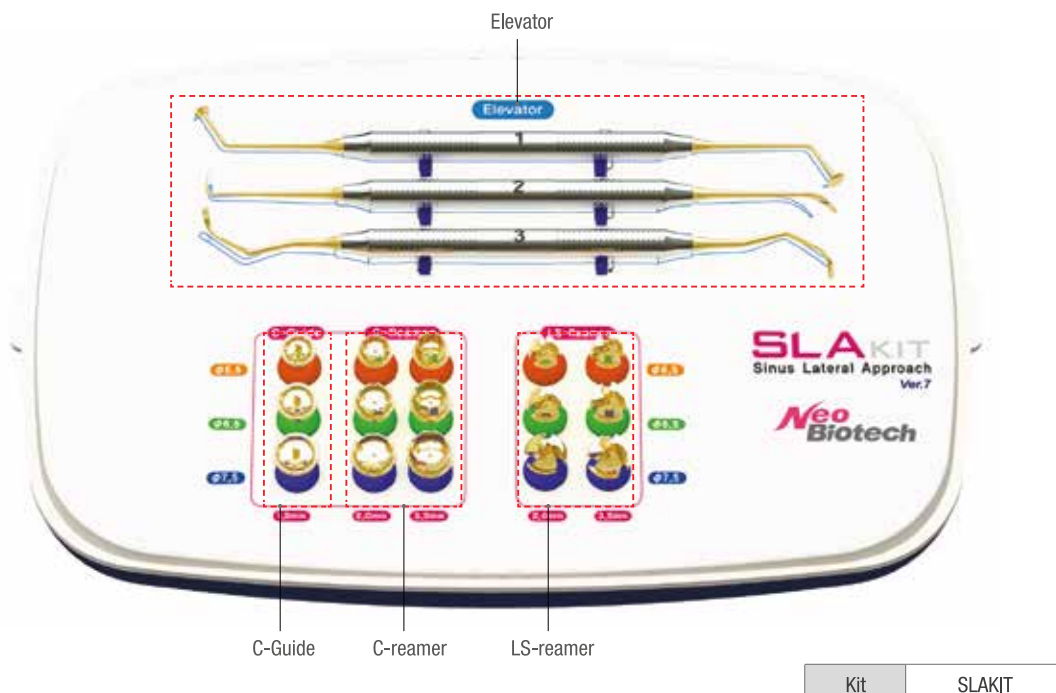

SCA Kit (Sinus Crestal Approach Kit)

• Sinus Crestal Approach Kit Intended use



1

Drilling

- Make drills 1mm shorter than measured height of residual bone. Drill only 1mm more in each step by step using 1mm longer stopper before the final drilling.



2

Using S-reamer

- For safety, select a proper S-reamer in diameter and 1mm shorter than measured height of remained bone. And make drills.
- If the sinus inferior cortical wall doesn't perforate until the stopper reaches to the crestal bone, change 1mm longer size stopper and drilling continuously.
- You can feel perforating in inferior cortical wall.



3

Check perforation

- Using Depth Gauge, check whether being perforated. Then, hang on the end of depth gauge in sinus wall inside. And check whether the tip side of gauge is hung on the interior wall.



4

Bone carrier

- Carry the bone grafting materials into osteotome site.
- One time insertion capacity 0.05cc.
- To make 1mm graft height, 0.1cc is needed.



5

Bone condenser

- Push and keep the graft materials in place on the floor of the sinus through the osteotome site.



6

Bone inserter

- Push the bone into sinus after inserting the bone into a hole with bone carrier.
- Can be safely used with 1mm long stopper. 80rpm speed.



7

Bone spreader

- Spreading the bone and reduce pressure in sinus area. 80rpm speed.
- Use bone spreader at least after inserting the bone more than 2 times.




8

Final Drilling & Implantation

- Do a Final Drilling.
- Based on the density of Crestal cortical bone, the Countersink should be done (Except IT Type of Fixture). Generally, it should be done for D1-D2 bone. But, in case of below of D3 bone, it is Okay to skip according to the decision of dentist.
- After finishing a whole of drilling, do a implantation.

FR Kit (Fixture Remover Kit)

This product is a surgical tool designed to remove implants that were stopped during the implantation due to torque or implants whose surrounding bones have been damaged. After removing the implant, a new implant with the same diameter can be immediately implanted.

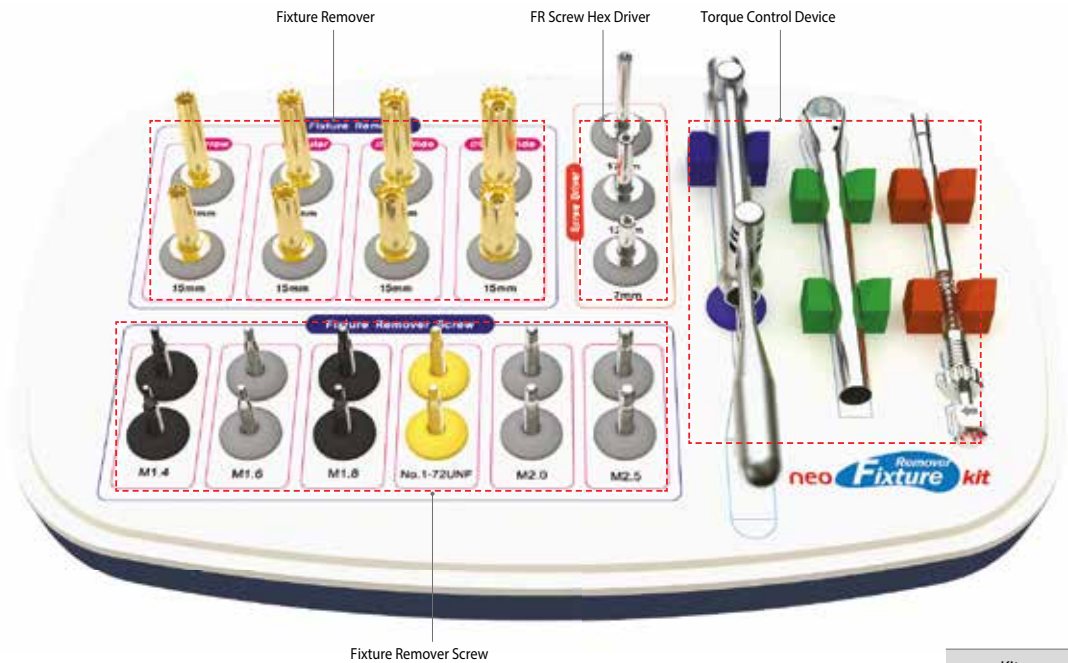

Kit	FRKIT
-----	-------

• Fixture Remover Screw




Screw size	Product Name	Recommended Torque (Ncm)
M1.4	FRS14	60
M1.6	FRS16	80
M1.8	FRS18	80
1-72UNF	FRS172	80
M2.0	FRS20	80
M2.5	FRS25	80




* "M" means a metric screw, and the number stands for the size of the external diameter of the screw

• FR Screw Hex Driver



Length	Product name
7mm	HDF1607
12mm	HDF1612
17mm	HDF1617




FR Kit (Fixture Remover Kit)

• Fixture Remover




Type	Length	Product name
Narrow	15mm	FR315
	20mm	FR320
Regular	15mm	FR415
	20mm	FR420
Wide(Ø5)	15mm	FR515
	20mm	FR520
Wide(Ø6~8)	15mm	FR615
	20mm	FR620

• Fixture removing Torque



Fixture size	Remover	Screw	Maximum Torque (Ncm)
Narrow	FR315 or FR320	FRS14	200
		FRS16	250
		FRS18/FRS172	300
		FRS20	350
Regular	FR315 or FR320	FRS18/FRS172	300
		FRS20	350
	FR415 or FR420	FRS18/FRS172	300
		FRS20	350
Wide(Ø5)	FR415 or FR420	FRS20	350
		FRS25	400
	FR515 or FR520	FRS20	350
		FRS25	400
Wide(Ø6~8)	FR515 or FR520	FRS20	350
		FRS25	400
	FR615 or FR620	FRS20	350
		FRS25	400

• Torque Control Device

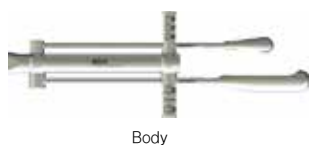

Body



Slider

Type	Product name
Body	TW80400
Slider	FRCHT

FR Kit (Fixture Remover Kit)

• Fixture Remover Kit Technique Guide



1 Failed implant

- Completely remove the prosthesis of the implant that needs to be removed.



2 Fixture Remover Screw

- Select an appropriate size of Fixture Remover Screw
- Connect the Fixture Remover Screw to the FR Screw Hex Driver and tighten it clockwise.



3 Fixture Remover


- Select an appropriate size of Fixture Remover
- Connect the selected Fixture Remover and tighten it counterclockwise until it is completely tightened to the Fixture Remover Screw that is fixed in the implant.
- Using a Torque Wrench, further apply torque to the Fixture Remover (counterclockwise) until the implant is finally unscrewed from the site.



4 Clear

SR Kit (Screw Remover Kit)

This product is a surgical tool developed in order safely and quickly to remove screws that have become fractured inside an implanted Fixture for various reasons. After removing the Screw, a new Abutment may be connected to the Fixture.

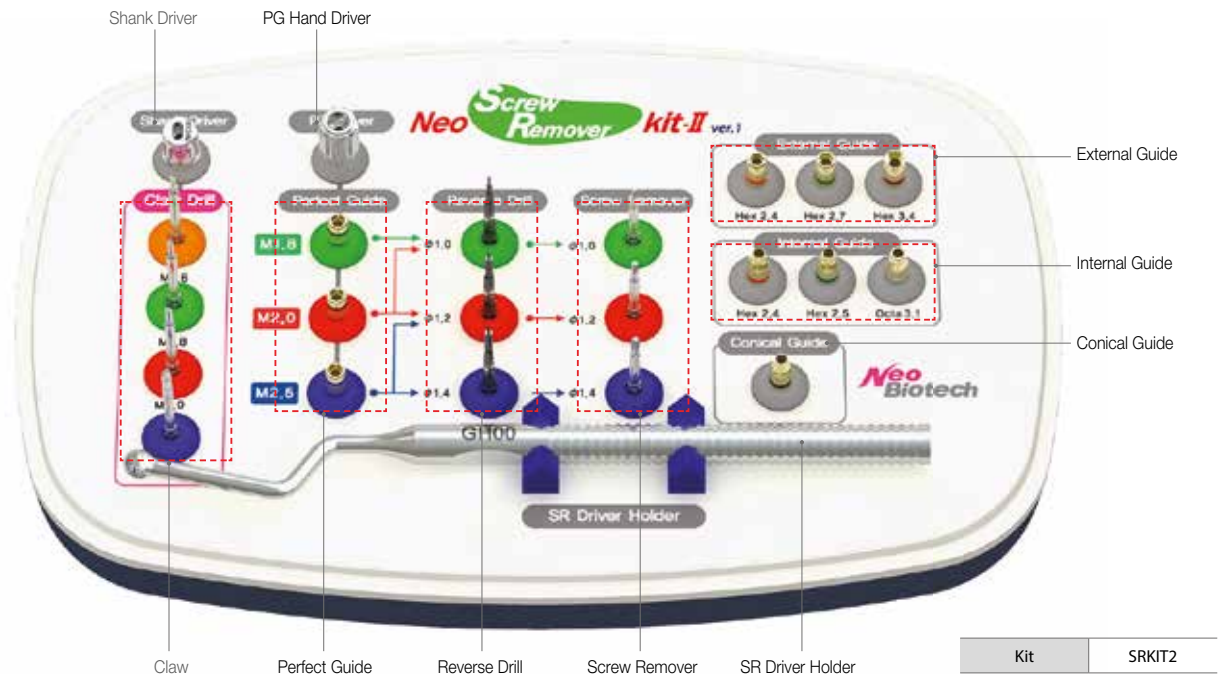


Kit	SRKIT2
-----	--------

• Claw



Fractured Screw size	Product name
M1.6	CD16
M1.8	CD18
M2.0	CD20
M2.5	CD25

* 80rpm



• Reverse Drill



Fractured Screw size	Diameter	Product name
M1.8	Ø1.0	RCD10
M2.0	Ø1.2	RCD12
M2.5	Ø1.4	RCD14

* For M1.6 Size Screw, use the claw for removal/2,000 rpm


SR Kit (Screw Remover Kit)

• Screw Remover



Fractured Screw size	Diameter	Product name
M1.8	Ø1.0	SR10
M2.0	Ø1.2	SR12
M2.5	Ø1.4	SR14


* At or below 80 rpm



• Shank Driver



Applicable Products	Standard	Product Name
Screw Remover (SR10, SR12, SR14)	for Hand or Ratchet	SHD00



• Perfect Guide & PG Hand Driver




Perfect Guide

Applicable Revers Drill	Fractured Screw size	Diameter (Ø)	Product Name
RCD10	M1.8	Ø1.0	PG1018
RCD10, RCD12	M1.8, M2.0	Ø1.2	PG1220
RCD12, RCD14	M2.0, M2.5	Ø1.4	PG1425

PG Hand Driver

Applicable Products	Standard	Product Name
Screw Remover (PG1018, PG1220, PG1425)	2.5Hex	PGHD25SS



SR Kit (Screw Remover Kit)

• Conical, Internal, External Guide



Conical Guide

Applicable Products	Standard	Product Name
Having 11° / 8° Internal Fixture	11° / 8°	CG00



Internal Guide

Applicable fixture	Standard	Product Name
Having 2.4Hex Internal Connection Fixture	2.4Hex	IHG24
M2.0 Having 2.5Hex Internal Connection Fixture	2.5Hex	IHG25
Having 3.1Octa Internal Connection Fixture	3.1Octa	IOG31




External Guide

Applicable fixture	Standard	Product Name
Having 2.4Hex External Connection Fixture	2.4Hex	EHG24
Having 2.7Hex External Connection Fixture	2.7Hex	EHG27
Having 3.4Hex External Connection Fixture	3.4Hex	EHG34

• SR Driver Holder



Applicable Products	Standard	Product Name
Conical Guide : CG00	2.4Hex	GH00
Internal Guide : IHG24, IHG25, IOG31		
External Guide : EHG24, EHG27, EHG34		



SR Kit (Screw Remover Kit)

• Screw Remover Kit Technique Guide



1 Fractured screw



2 Perfect Guide

- Select an appropriate size of Perfect Guide
- By using the PG Hand Driver, tighten the Perfect Guide to the Fixture in a clockwise direction until it touches the screw inside the fixture.



3 Reverse Drill

- Select an appropriate size of Reverse Drill and connect it to the contra angle of the surgical engine.
- Insert the Reverse Drill into the Perfect Guide attached on the fixture.
- By drilling counterclockwise at a speed of approximately 2000rpm, drill 1~2mm into the surface of the fractured screw.
- Check the marking line (in 1mm intervals) of the Drill body while drilling with adequate irrigation.




4 Screw RemoverClear

- Remove the Perfect guide connected to the Fixture
- Select a Screw Remover that fits to the hole created by the Reverse Drill.
- Connect the Screw Remover to the contra angle of surgical engine and drill slowly (less than 80rpm) while pressing down with enough force to remove the fractured screw.

ACM (Auto Chip Maker)

ACM is an instrument to collect autograft bone from mandibular molars or incisor for GBR in defected area.

• Auto Chip Maker

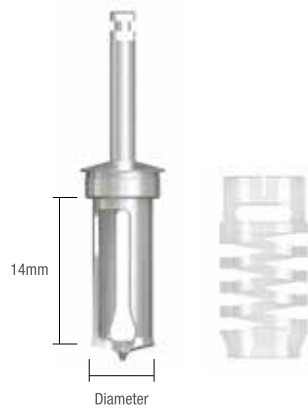

Diameter (Ø)	Product name
Ø 4.0	NACM40ISETS
Ø 4.5	NACM45ISETS
Ø 5.0	NACM50ISETS
Ø 6.0	NACM60ISETS

* ACM Stopper 7ea Included

• Auto Chip Maker Technique Guide



Stopper

- Connect the stopper to the sterilized ACM drill. .



Locate the ACM

- Select the most suitable place to collect autograft bone.
- Position the ACM Drill where the autograft bone will be collected.



Drilling

- To prevent slipping of the ACM drill, slightly tilt the drill left and right until the drill stably positions itself. (80rpm / Non-irrigation recommended)
- In order to collect high quality autograft bone, drill only 3~4mm deep from on site, and move on to a different site to continue drilling.



Peri-implantitis Solution


• i-Brush 1




Product name	IBRUSH1
--------------	---------



• i-Brush 2




Product name	IBRUSH 2
--------------	----------

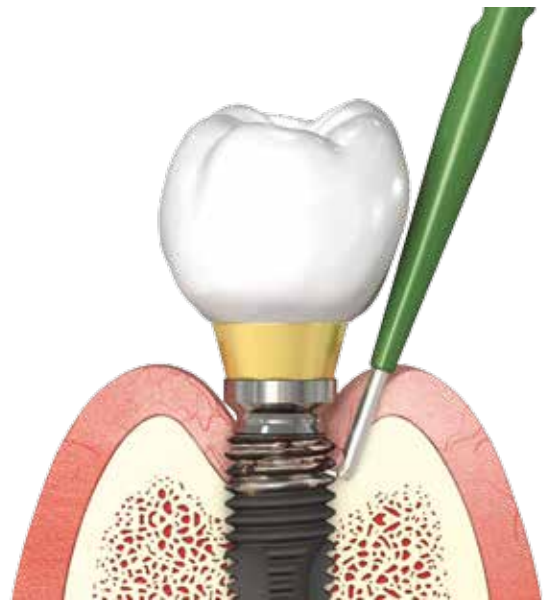

• R-Brush



Product Code	
Regular (Ø5.6)	ROUND BRUSH (R)
Wide (Ø6.6)	ROUND BRUSH (W)

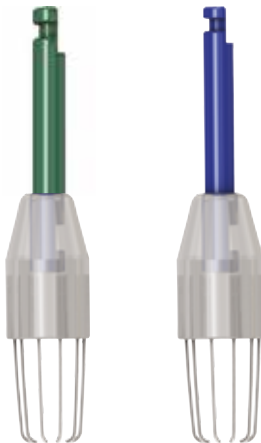



Find Neobiotech online

AnyCheck

2017.10 E-Ver.02

Dental implant stability meter (tapping-motion) for assessing osseointegration without disconnecting the healing abutment.



Measured value is similar to ISQ scale: above 60 – bridge recommended; above 70 – single case loading possible.

Displayed in **red** – 30~59 ; **orange** – 60~64 ; **green** – 65~85.

Measured values (IST scale) differ depending on the height of the healing abutment. As the standard height of the healing abutment is 4mm, calculate the correct IST value according to the following chart:

Standard +3	7mm height Healing Abutment	Displayed IST value +6
Standard +2	6mm height Healing Abutment	Displayed IST value +4
Standard +1	5mm height Healing Abutment	Displayed IST value +2
Standard	4mm height Healing Abutment	Displayed IST value
Standard - 1	3mm height Healing Abutment	Displayed IST value - 2
Standard - 2	2mm height Healing Abutment	Displayed IST value - 4
Standard - 3	1mm height Healing Abutment	Displayed IST value - 6



NeoBiotech Implant System

DISTRIBUITO DA



Butterfly Italia s.r.l.

Via I° Maggio, 1 - 20873 Cavenago di Brianza (MB)

Tel. +39 02 95335246

info@butterflyitalia.com - www.butterflyitalia.com 

Neo
Biotech
Satisfaction to Dentists

Neobiotech Co., Ltd. E-space #1001,36, Digital-ro 27-gil, Guro-gu, Seoul, Republic of Korea
Tel. +82-2-582-2885 Fax. +82-2-582-2883